

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016839.D
 Acq On : 29 Aug 2023 19:03
 Operator : MA/JU
 Sample : 04134-08
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCHK1

Quant Time: Aug 29 23:20:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 29 01:12:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.028	152	305759	20.000	ng/ul	0.00
20) Naphthalene-d8	10.857	136	1389568	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.681	164	878802	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.445	188	1946347	20.000	ng/ul	-0.01
79) Chrysene-d12	21.545	240	1485253	20.000	ng/ul	0.00
88) Perylene-d12	24.115	264	1328691	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	40376	5.458	ng/uL	0.00
4) Pyridine-d5	3.816	84	215519	9.533	ng/ul	0.00
7) Phenol-d5	7.169	99	194970	7.171	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.363	67	611367	35.281	ng/ul	0.00
11) 2-Chlorophenol-d4	7.546	132	542186	26.523	ng/ul	0.00
15) 4-Methylphenol-d8	8.728	113	367233	16.546	ng/ul	0.00
21) Nitrobenzene-d5	9.222	128	352093	33.512	ng/ul	0.00
24) 2-Nitrophenol-d4	9.940	143	329811	29.781	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.463	165	632591	30.639	ng/ul	0.00
31) 4-Chloroaniline-d4	11.010	131	723458	22.849	ng/ul	0.00
46) Dimethylphthalate-d6	14.092	166	2421664	36.540	ng/ul	0.00
49) Acenaphthylene-d8	14.381	160	2750028	36.706	ng/ul	0.00
54) 4-Nitrophenol-d4	14.886	143	49456	3.610	ng/ul	0.00
60) Fluorene-d10	15.675	176	2193959	39.311	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.798	200	243708	21.025	ng/ul	0.00
73) Anthracene-d10	17.545	188	3604857	41.784	ng/ul	-0.01
81) Pyrene-d10	19.780	212	4044527	49.582	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.945	264	2825774	42.457	ng/ul	0.00
Target Compounds						
71) Pentachlorophenol	17.075	266	30246	1.950	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016839.D
Acq On : 29 Aug 2023 19:03
Operator : MA/JU
Sample : 04134-08
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHK1

Quant Time: Aug 29 23:20:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 29 01:12:28 2023
Response via : Initial Calibration

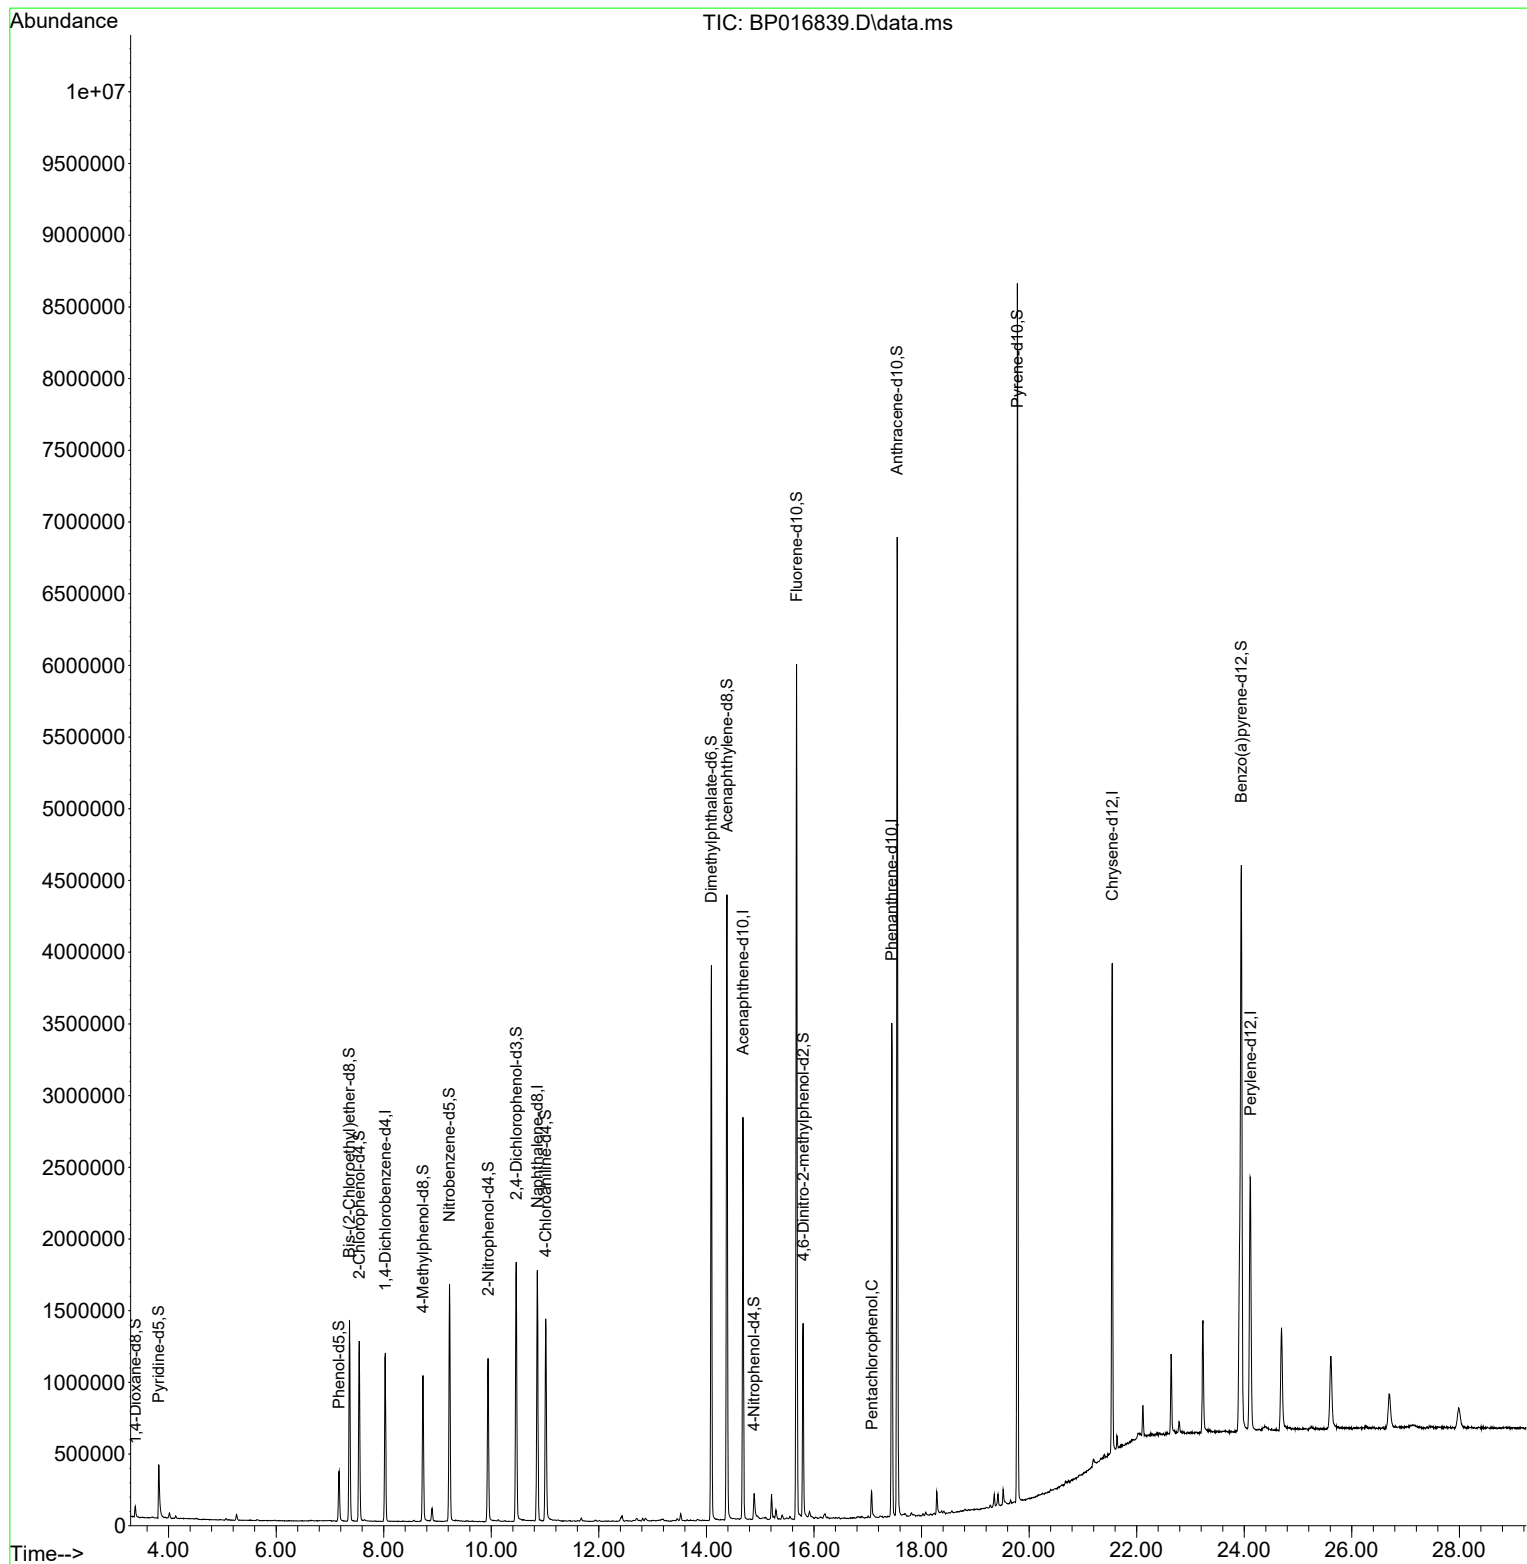

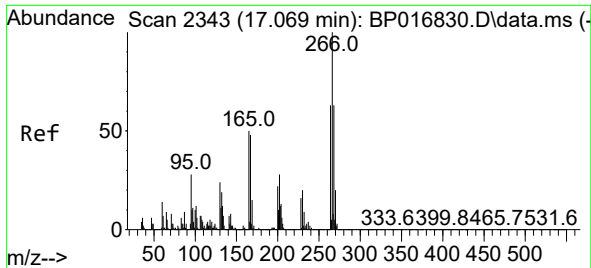

#71
 Pentachlorophenol
 Concen: 1.950 ng/ul
 RT: 17.075 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BP016839.D
 Acq: 29 Aug 2023 19:03

Instrument :
 BNA_P
 ClientSampleId :
 DCHK1

Tgt Ion:266 Resp: 30246
 Ion Ratio Lower Upper
 266 100
 264 63.0 50.7 76.1
 268 62.2 50.8 76.2

