

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016848.D
 Acq On : 30 Aug 2023 00:11
 Operator : MA/JU
 Sample : 04148-08
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJX2

Quant Time: Aug 30 01:08:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 29 01:12:28 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.028	152	419318	20.000	ng/u1	0.00
20) Naphthalene-d8	10.851	136	1859415	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.681	164	1170567	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.445	188	2491355	20.000	ng/u1	-0.01
79) Chrysene-d12	21.539	240	1703964	20.000	ng/u1	-0.01
88) Perylene-d12	24.110	264	1547018	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	50615	4.989	ng/uL	0.00
4) Pyridine-d5	3.817	84	312533	10.080	ng/u1	0.00
7) Phenol-d5	7.169	99	315616	8.465	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.363	67	863625	36.342	ng/u1	0.00
11) 2-Chlorophenol-d4	7.546	132	817495	29.161	ng/u1	0.00
15) 4-Methylphenol-d8	8.728	113	581949	19.119	ng/u1	0.00
21) Nitrobenzene-d5	9.222	128	534061	37.987	ng/u1	0.00
24) 2-Nitrophenol-d4	9.940	143	553465	37.348	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.463	165	968766	35.065	ng/u1	0.00
31) 4-Chloroaniline-d4	11.010	131	593793	14.015	ng/u1	0.00
46) Dimethylphthalate-d6	14.092	166	3574229	40.489	ng/u1	0.00
49) Acenaphthylene-d8	14.381	160	3856659	38.646	ng/u1	0.00
54) 4-Nitrophenol-d4	14.887	143	102959	5.643	ng/u1	0.00
60) Fluorene-d10	15.675	176	3006347	40.441	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.798	200	459559	30.974	ng/u1	0.00
73) Anthracene-d10	17.545	188	4882054	44.209	ng/u1	-0.01
81) Pyrene-d10	19.780	212	5210037	55.672	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.939	264	3452804	44.557	ng/u1	-0.01
Target Compounds						
2) 1,4-Dioxane	3.417	88	84160	7.617	ng/uL	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016848.D
Acq On : 30 Aug 2023 00:11
Operator : MA/JU
Sample : 04148-08
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJX2

Quant Time: Aug 30 01:08:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 29 01:12:28 2023
Response via : Initial Calibration

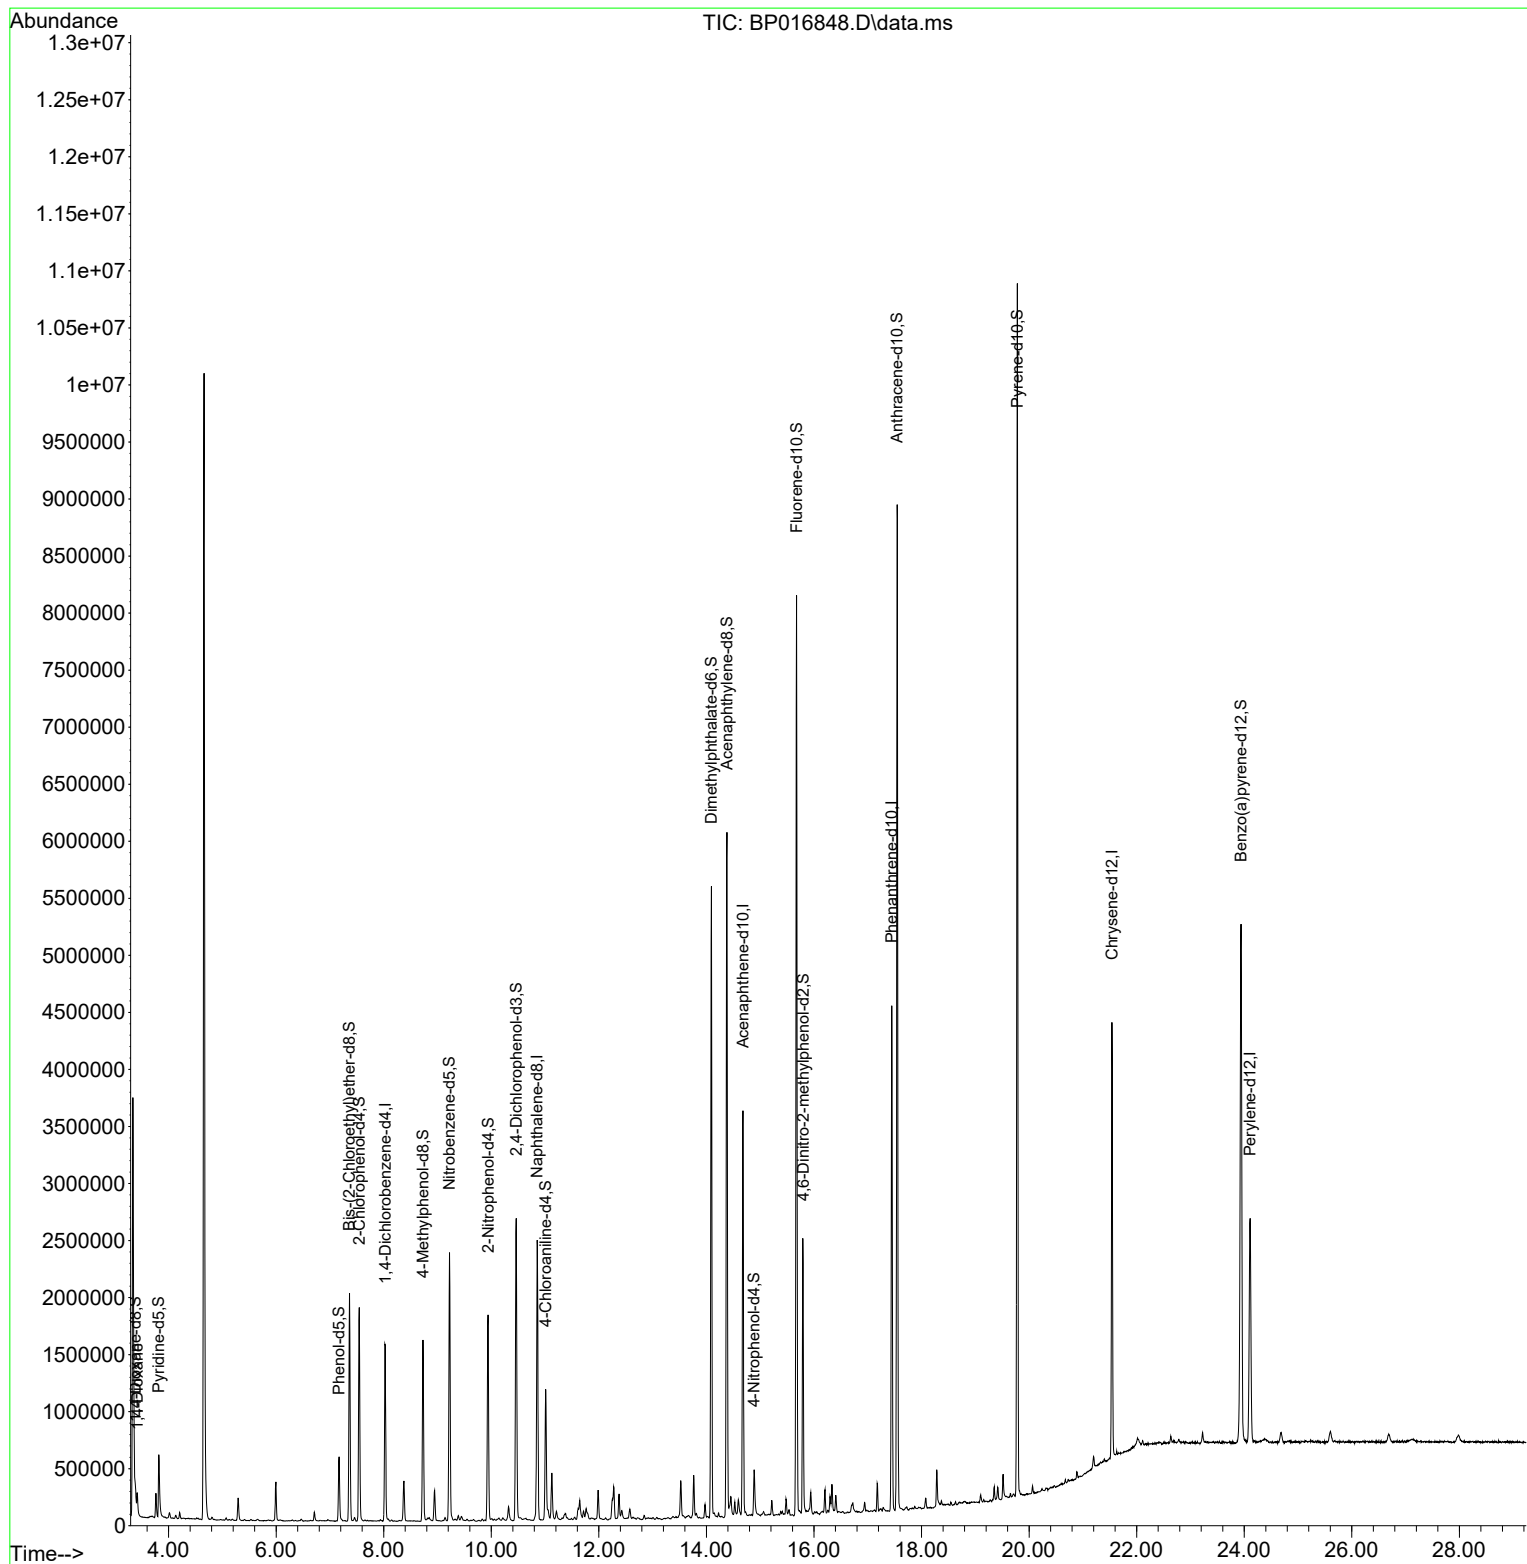

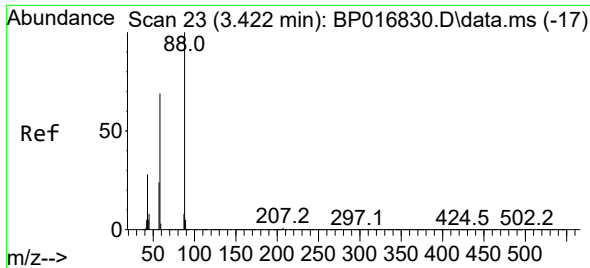

#2
 1,4-Dioxane
 Concen: 7.617 ng/uL
 RT: 3.417 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BP016848.D
 Acq: 30 Aug 2023 00:11

Instrument :
 BNA_P
 ClientSampleId :
 BBJX2

Tgt Ion: 88 Resp: 84160
 Ion Ratio Lower Upper
 88 100
 43 32.4 24.0 36.0
 58 77.4 59.8 89.8

