

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016853.D
 Acq On : 30 Aug 2023 03:34
 Operator : MA/JU
 Sample : 04148-10
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBKG5

Quant Time: Aug 30 04:22:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 30 02:25:00 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.022	152	424234	20.000	ng/u1	0.00
20) Naphthalene-d8	10.852	136	1892683	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.675	164	1174803	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.445	188	2513433	20.000	ng/u1	0.00
79) Chrysene-d12	21.539	240	1798164	20.000	ng/u1	0.00
88) Perylene-d12	24.110	264	1614775	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	50975	4.966	ng/uL	0.00
4) Pyridine-d5	3.817	84	276715	8.822	ng/u1	0.00
7) Phenol-d5	7.169	99	306123	8.115	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.364	67	932973	38.805	ng/u1	0.00
11) 2-Chlorophenol-d4	7.546	132	867089	30.571	ng/u1	0.00
15) 4-Methylphenol-d8	8.728	113	609379	19.788	ng/u1	0.00
21) Nitrobenzene-d5	9.222	128	583721	40.790	ng/u1	0.00
24) 2-Nitrophenol-d4	9.940	143	606754	40.224	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.457	165	1079240	38.378	ng/u1	0.00
31) 4-Chloroaniline-d4	11.010	131	438322	10.164	ng/u1	0.00
46) Dimethylphthalate-d6	14.093	166	4046753	45.676	ng/u1	0.00
49) Acenaphthylene-d8	14.381	160	4415351	44.085	ng/u1	0.00
54) 4-Nitrophenol-d4	14.887	143	102211	5.582	ng/u1	0.00
60) Fluorene-d10	15.675	176	3463930	46.428	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.798	200	548800	36.664	ng/u1	0.00
73) Anthracene-d10	17.545	188	5654491	50.754	ng/u1	0.00
81) Pyrene-d10	19.781	212	6097410	61.741	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.939	264	4170385	51.559	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.417	88	31705	2.836	ng/uL	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016853.D
Acq On : 30 Aug 2023 03:34
Operator : MA/JU
Sample : 04148-10
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBKG5


Quant Time: Aug 30 04:22:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 30 02:25:00 2023
Response via : Initial Calibration

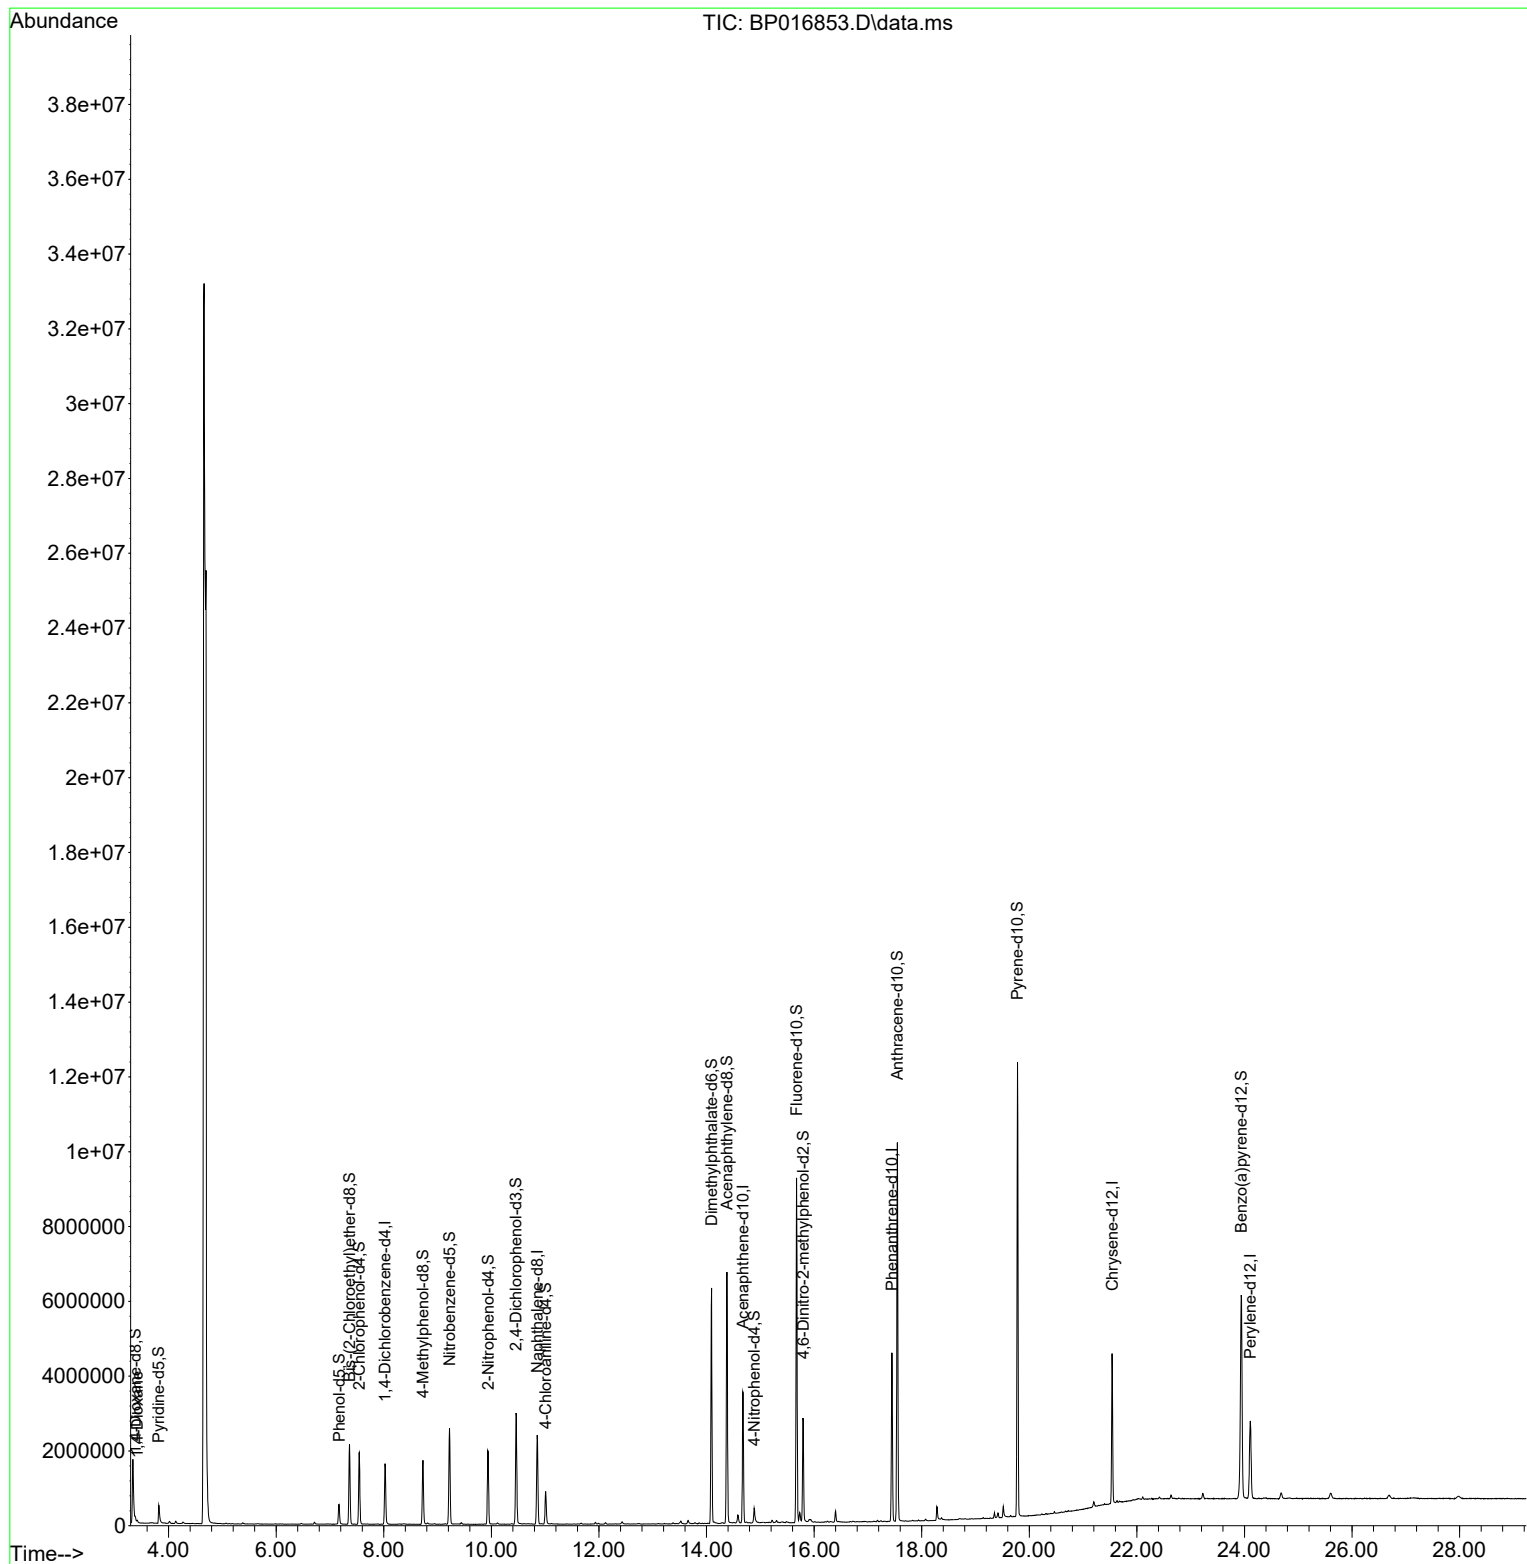

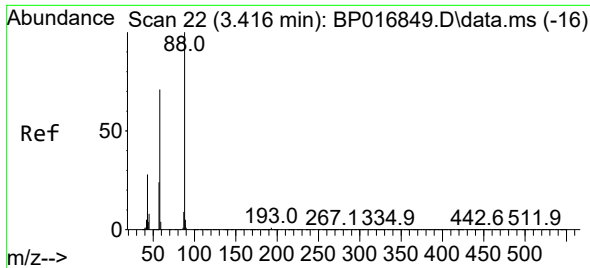

#2
 1,4-Dioxane
 Concen: 2.836 ng/uL
 RT: 3.417 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BP016853.D
 Acq: 30 Aug 2023 03:34

Instrument :
 BNA_P
 ClientSampleId :
 BBKG5

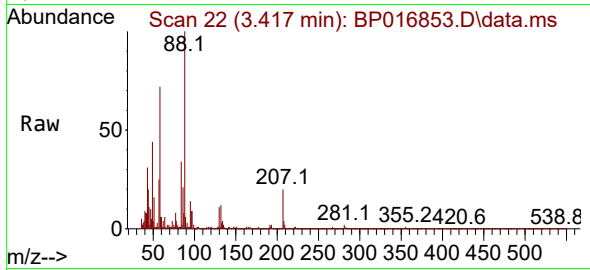

Tgt Ion: 88 Resp: 31705
 Ion Ratio Lower Upper
 88 100
 43 30.6 24.0 36.0
 58 72.2 59.8 89.8

