

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016855.D
 Acq On : 30 Aug 2023 04:42
 Operator : MA/JU
 Sample : 04148-12
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJW5

Quant Time: Aug 30 05:13:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 30 02:25:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.022	152	459966	20.000	ng/u1	0.00
20) Naphthalene-d8	10.852	136	2032967	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.675	164	1252421	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.445	188	2631228	20.000	ng/u1	0.00
79) Chrysene-d12	21.539	240	1816901	20.000	ng/u1	0.00
88) Perylene-d12	24.110	264	1705408	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	58074	5.218	ng/uL	0.00
4) Pyridine-d5	3.817	84	354782	10.432	ng/u1	0.00
7) Phenol-d5	7.164	99	323582	7.911	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.364	67	1043387	40.026	ng/u1	0.00
11) 2-Chlorophenol-d4	7.546	132	936457	30.452	ng/u1	0.00
15) 4-Methylphenol-d8	8.728	113	623008	18.659	ng/u1	0.00
21) Nitrobenzene-d5	9.222	128	638828	41.560	ng/u1	0.00
24) 2-Nitrophenol-d4	9.940	143	655216	40.439	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.458	165	1122400	37.158	ng/u1	0.00
31) 4-Chloroaniline-d4	11.010	131	521007	11.247	ng/u1	0.00
46) Dimethylphthalate-d6	14.093	166	4056673	42.951	ng/u1	0.00
49) Acenaphthylene-d8	14.381	160	4526314	42.392	ng/u1	0.00
54) 4-Nitrophenol-d4	14.887	143	91181	4.671	ng/u1	0.00
60) Fluorene-d10	15.675	176	3452114	43.402	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.793	200	515482	32.897	ng/u1	0.00
73) Anthracene-d10	17.545	188	5329979	45.700	ng/u1	0.00
81) Pyrene-d10	19.781	212	5625653	56.376	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.939	264	3947936	46.215	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.417	88	19442	1.604	ng/uL	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016855.D
Acq On : 30 Aug 2023 04:42
Operator : MA/JU
Sample : 04148-12
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJW5

Quant Time: Aug 30 05:13:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 30 02:25:00 2023
Response via : Initial Calibration

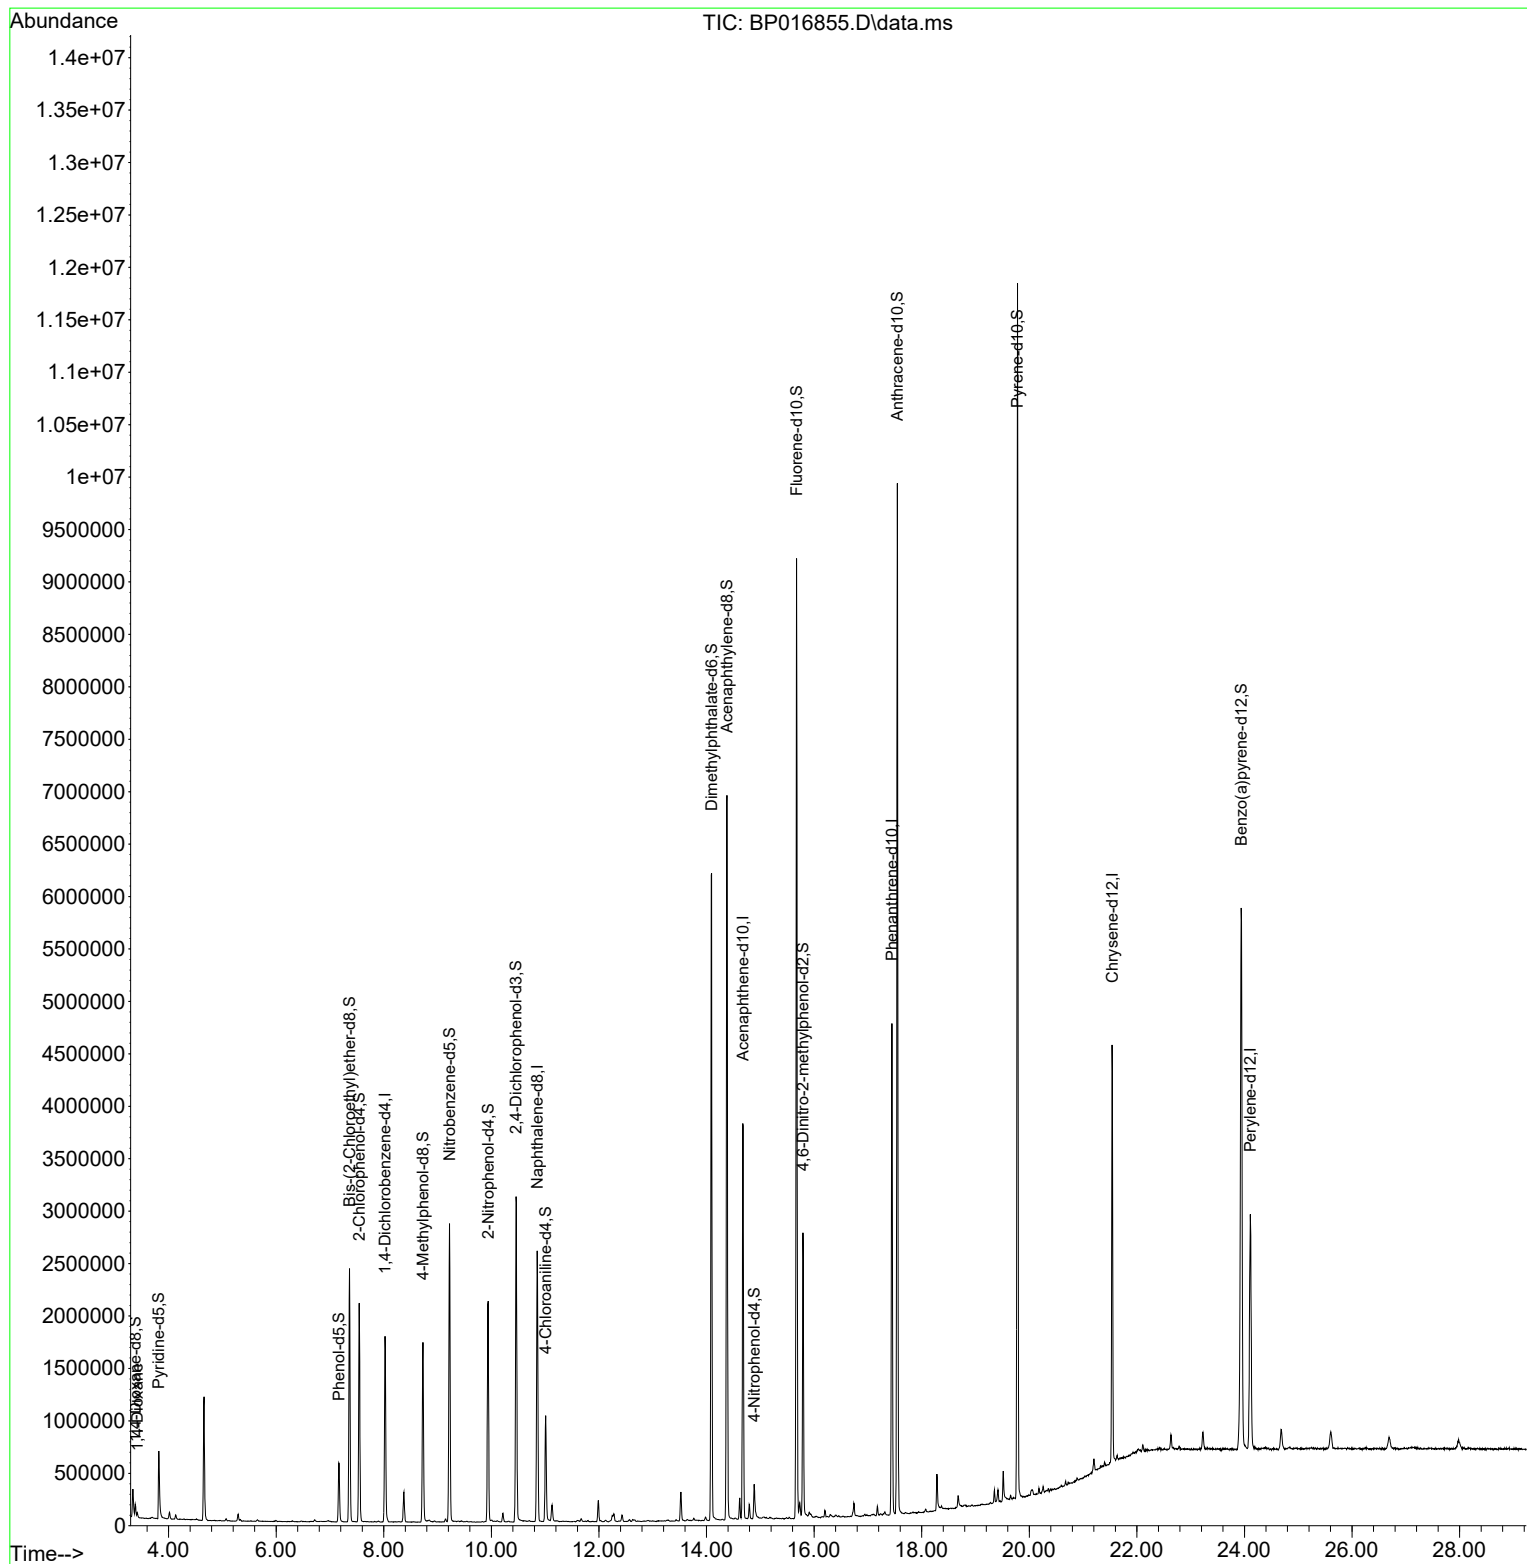

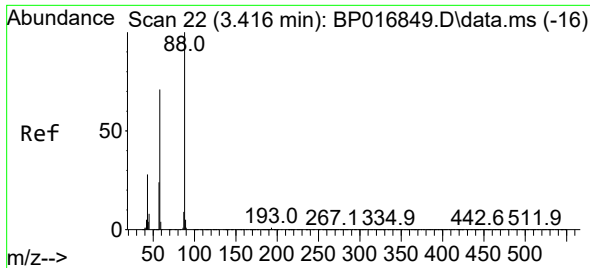

#2
 1,4-Dioxane
 Concen: 1.604 ng/uL
 RT: 3.417 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BP016855.D
 Acq: 30 Aug 2023 04:42

Instrument :
 BNA_P
 ClientSampleId :
 BBJW5

Tgt Ion: 88 Resp: 19442
 Ion Ratio Lower Upper
 88 100
 43 34.0 24.0 36.0
 58 74.0 59.8 89.8

