

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016866.D
 Acq On : 30 Aug 2023 10:56
 Operator : MA/JU
 Sample : 04123-20
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAU0

Quant Time: Aug 31 00:48:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 30 02:25:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.022	152	459816	20.000	ng/u1	0.00
20) Naphthalene-d8	10.851	136	2012269	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.674	164	1234677	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.445	188	2709369	20.000	ng/u1	0.00
79) Chrysene-d12	21.539	240	2251911	20.000	ng/u1	0.00
88) Perylene-d12	24.109	264	2105034	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	88735	7.976	ng/uL	0.00
4) Pyridine-d5	3.810	84	744059	21.885	ng/u1	0.00
7) Phenol-d5	7.163	99	779601	19.067	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.363	67	1160714	44.541	ng/u1	0.00
11) 2-Chlorophenol-d4	7.540	132	1168792	38.020	ng/u1	0.00
15) 4-Methylphenol-d8	8.728	113	933723	27.975	ng/u1	0.00
21) Nitrobenzene-d5	9.222	128	718187	47.203	ng/u1	0.00
24) 2-Nitrophenol-d4	9.934	143	755866	47.131	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.457	165	1289166	43.118	ng/u1	0.00
31) 4-Chloroaniline-d4	11.010	131	1657846	36.157	ng/u1	0.00
46) Dimethylphthalate-d6	14.092	166	4233055	45.462	ng/u1	0.00
49) Acenaphthylene-d8	14.374	160	4891152	46.468	ng/u1	0.00
54) 4-Nitrophenol-d4	14.880	143	267630	13.906	ng/u1	0.00
60) Fluorene-d10	15.674	176	3701675	47.209	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.798	200	609566	37.779	ng/u1	0.00
73) Anthracene-d10	17.545	188	5948418	49.531	ng/u1	0.00
81) Pyrene-d10	19.780	212	6881945	55.644	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.945	264	5443499	51.625	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.416	88	19310	1.594	ng/uL	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016866.D
Acq On : 30 Aug 2023 10:56
Operator : MA/JU
Sample : 04123-20
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAU0

Quant Time: Aug 31 00:48:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 30 02:25:00 2023
Response via : Initial Calibration

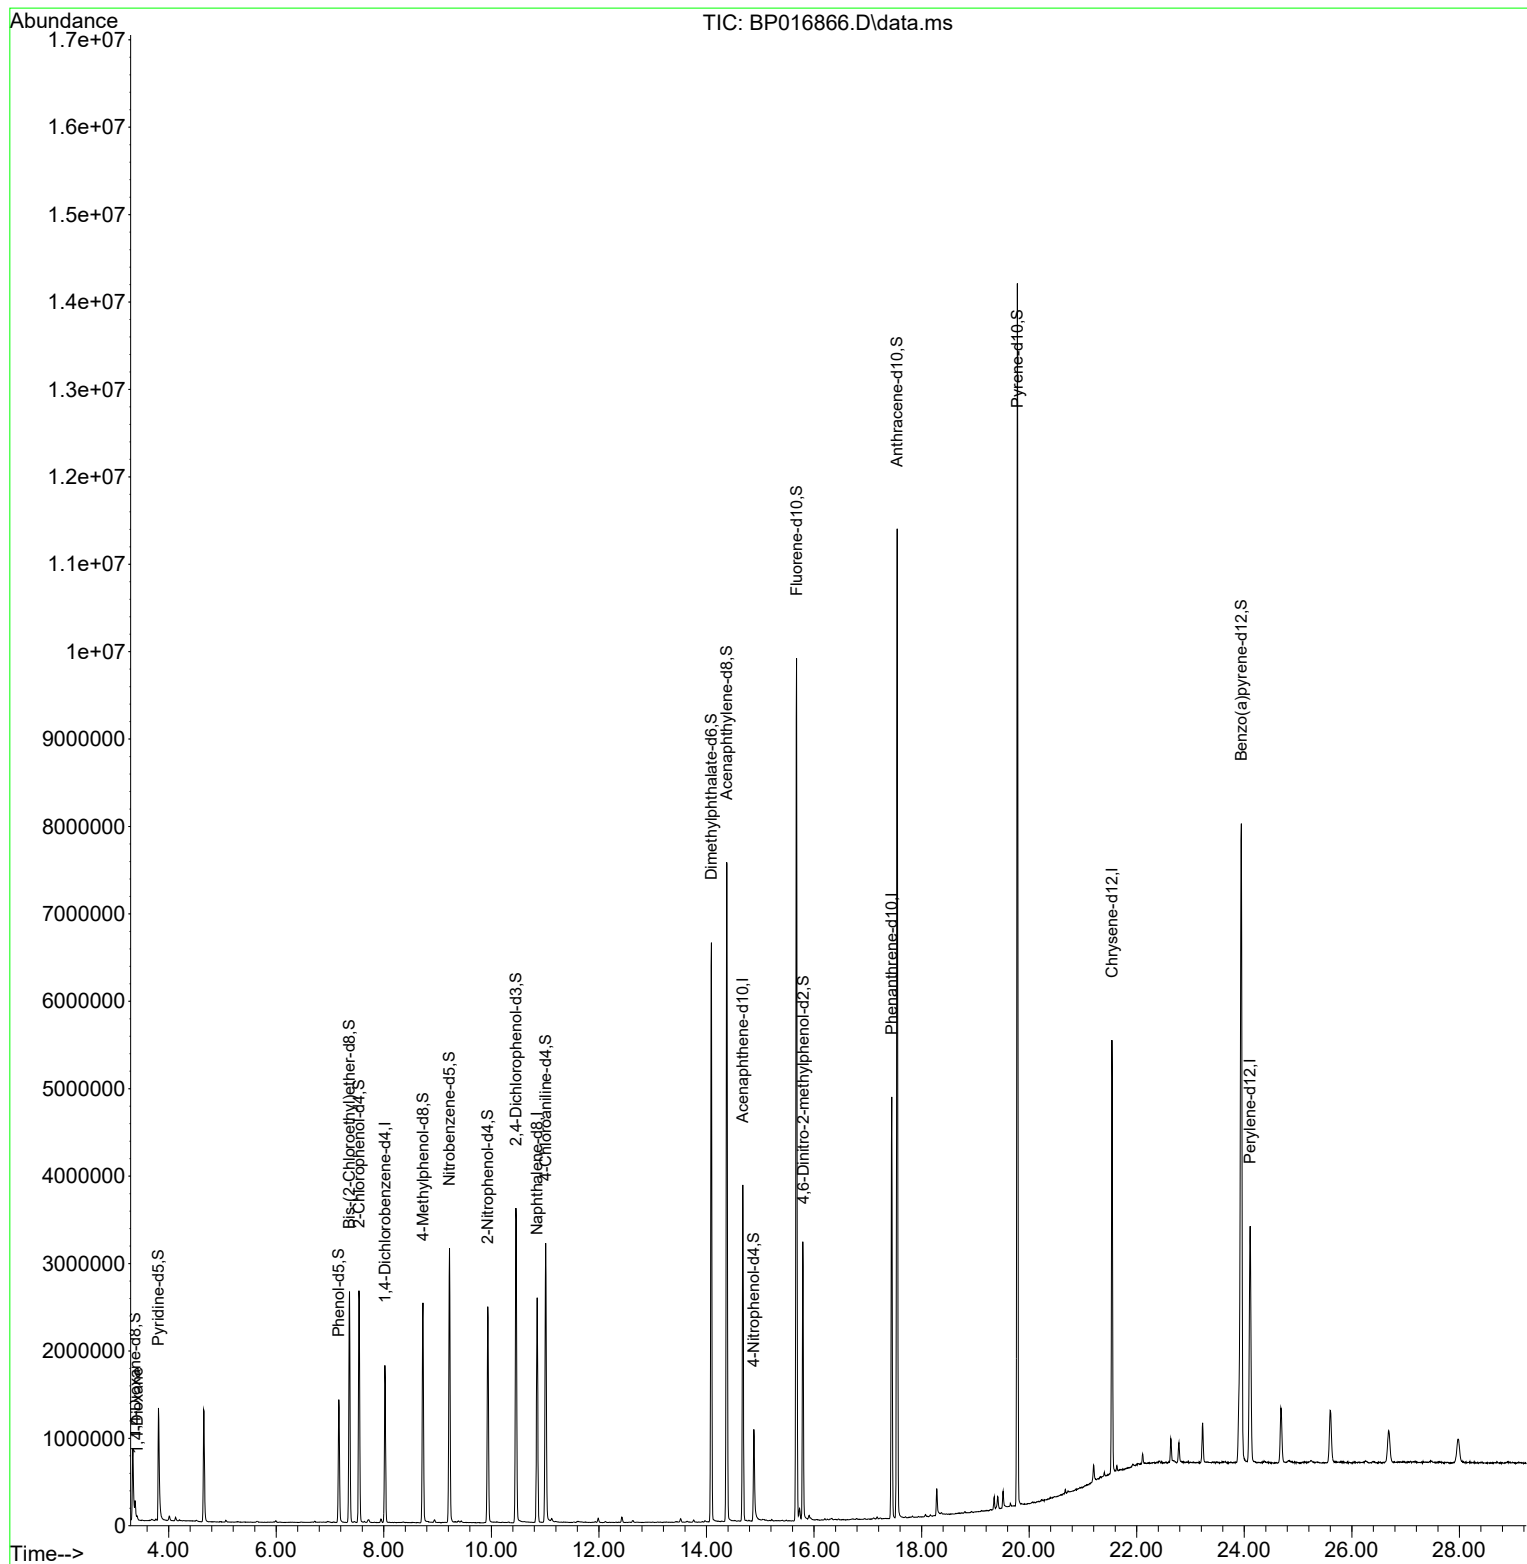

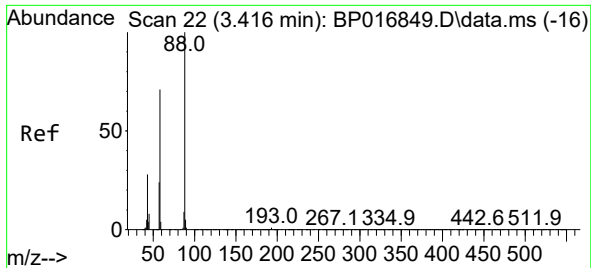

#2
 1,4-Dioxane
 Concen: 1.594 ng/uL
 RT: 3.416 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BP016866.D
 Acq: 30 Aug 2023 10:56

Instrument :
 BNA_P
 ClientSampleId :
 BHAU0

Tgt Ion: 88 Resp: 19310
 Ion Ratio Lower Upper
 88 100
 43 29.8 24.0 36.0
 58 77.1 59.8 89.8

