

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016787.D
 Acq On : 28 Aug 2023 11:04
 Operator : MA/JU
 Sample : PB155076BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK076

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016787.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	12	16	27	rVB	135933	209218	2.32%	0.220%
2	3.811	85	89	114	rBV	1379266	2239244	24.88%	2.354%
3	4.128	139	143	151	rVB	26359	42794	0.48%	0.045%
4	7.169	653	660	678	rBV	1653030	2603271	28.93%	2.736%
5	7.363	684	693	701	rBV	1372572	2095553	23.29%	2.203%
6	7.546	717	724	737	rBV	1599756	2509863	27.89%	2.638%
7	8.028	798	806	816	rBV	1397682	2167789	24.09%	2.279%
8	8.734	918	926	945	rBV	1971366	3221641	35.80%	3.386%
9	9.228	1002	1010	1021	rBV	1513892	2530792	28.12%	2.660%
10	9.940	1123	1131	1141	rBV	1231862	2027407	22.53%	2.131%
11	10.463	1212	1220	1237	rBV	1908291	3228168	35.87%	3.393%
12	10.857	1280	1287	1296	rBV	2013370	3365845	37.40%	3.538%
13	11.016	1306	1314	1335	rBV	1950675	3352867	37.26%	3.524%
14	12.439	1547	1556	1562	rBV	35164	62238	0.69%	0.065%
15	13.534	1735	1742	1747	rVB3	20860	35569	0.40%	0.037%
16	13.645	1755	1761	1766	rBV6	7434	11130	0.12%	0.012%
17	14.098	1831	1838	1851	rBV	3587426	4890344	54.34%	5.140%
18	14.386	1880	1887	1905	rBV	4200768	6073821	67.49%	6.384%
19	14.686	1930	1938	1953	rBV	3222662	4645658	51.62%	4.883%
20	14.892	1966	1973	1990	rBV	1203253	2146982	23.86%	2.257%
21	15.680	2100	2107	2122	rBV	5362583	7642236	84.92%	8.033%
22	15.804	2122	2128	2143	rVV	1260160	1767298	19.64%	1.858%
23	15.922	2144	2148	2157	rVB2	26288	47193	0.52%	0.050%
24	16.469	2237	2241	2246	rVB7	6307	12121	0.13%	0.013%
25	17.122	2349	2352	2356	rBV5	6667	9430	0.10%	0.010%
26	17.245	2369	2373	2381	rVB2	8289	17068	0.19%	0.018%
27	17.457	2402	2409	2419	rBV	4056226	5614350	62.39%	5.901%
28	17.557	2419	2426	2443	rVV	5756947	8219691	91.34%	8.639%
29	19.363	2729	2733	2738	rBV2	71962	93040	1.03%	0.098%
30	19.427	2741	2744	2751	rVB	54980	77498	0.86%	0.081%
31	19.792	2800	2806	2818	rBV	7135014	8999255	100.00%	9.459%
32	21.557	3101	3106	3115	rBV	3491338	4682794	52.04%	4.922%
33	23.962	3507	3515	3527	rVB2	3023365	6519644	72.45%	6.853%
34	24.133	3537	3544	3557	rVB	1847131	3979053	44.22%	4.182%

Sum of corrected areas: 95140865




Instrument :
BNA_P
ClientSampleId :
SBLK076

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016787.D
Acq On : 28 Aug 2023 11:04
Operator : MA/JU
Sample : PB155076BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK076

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

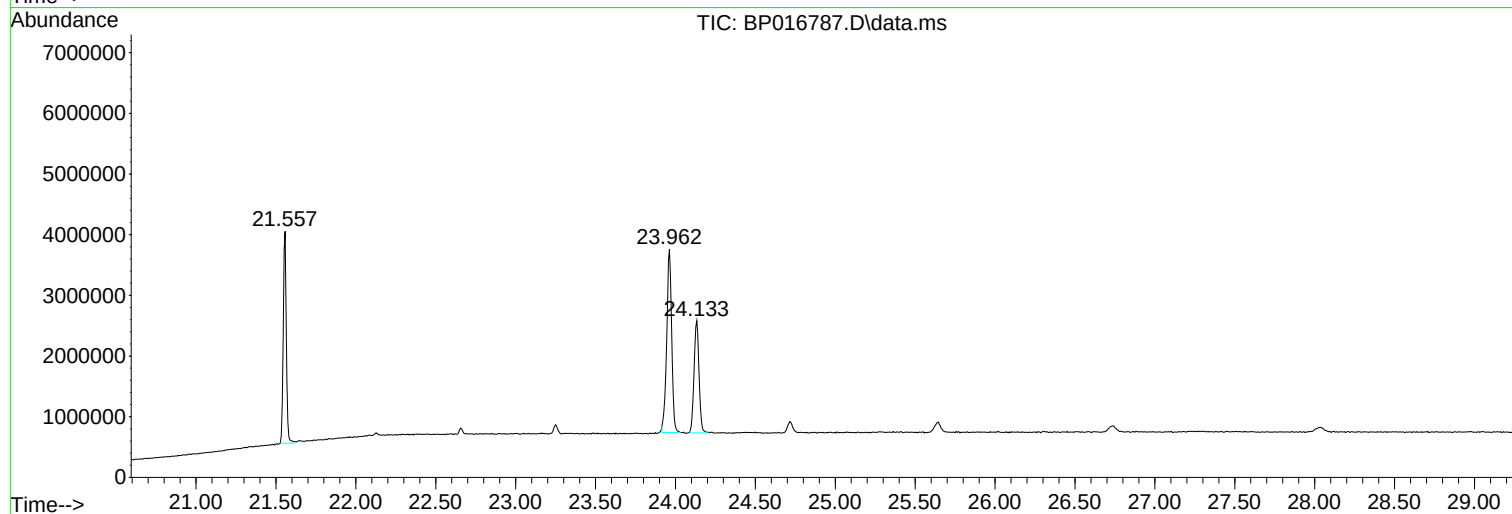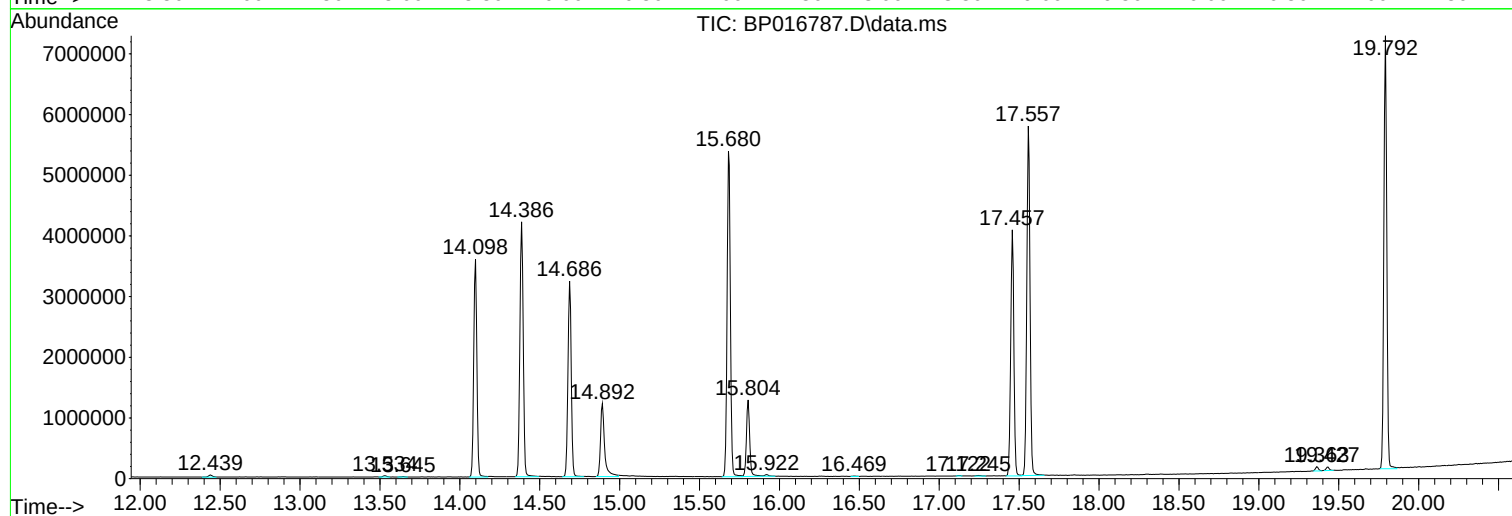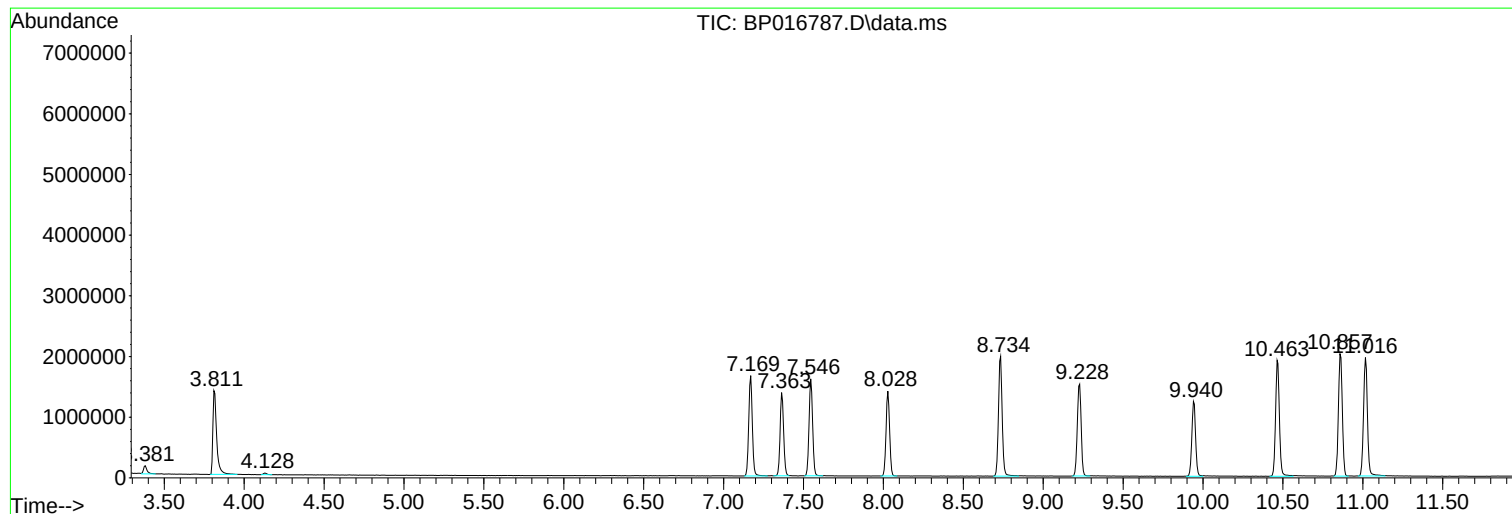

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016787.D
Acq On : 28 Aug 2023 11:04
Operator : MA/JU
Sample : PB155076BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK076

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016787.D
Acq On : 28 Aug 2023 11:04
Operator : MA/JU
Sample : PB155076BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK076

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc