

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016791.D
 Acq On : 28 Aug 2023 14:14
 Operator : MA/JU
 Sample : 04134-12
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCHK6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016791.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	13	17	34	rVB	101550	168253	1.44%	0.167%
2	3.822	87	91	109	rBV	548982	887956	7.61%	0.881%
3	4.022	120	125	130	rVB	48884	74379	0.64%	0.074%
4	4.134	140	144	154	rVB	23751	39955	0.34%	0.040%
5	4.658	230	233	240	rVB7	9824	17108	0.15%	0.017%
6	5.069	298	303	308	rBV	15374	25888	0.22%	0.026%
7	5.658	401	403	409	rVB3	8065	12414	0.11%	0.012%
8	7.169	651	660	672	rBV	433316	684581	5.87%	0.679%
9	7.369	685	694	703	rBV	1537020	2406680	20.63%	2.387%
10	7.546	717	724	734	rBV	1442201	2315475	19.85%	2.297%
11	8.028	799	806	818	rVB	1324123	2119967	18.18%	2.103%
12	8.734	919	926	942	rBV	1199398	1925329	16.51%	1.910%
13	9.228	1001	1010	1024	rBV	1845003	2952363	25.31%	2.929%
14	9.946	1122	1132	1151	rBV	1360517	2324207	19.93%	2.306%
15	10.463	1212	1220	1233	rBV	2005976	3358404	28.79%	3.331%
16	10.857	1280	1287	1294	rBV	1909799	3262969	27.97%	3.237%
17	10.910	1294	1296	1302	rVB	38076	50691	0.43%	0.050%
18	11.016	1305	1314	1335	rBV	2000010	3421689	29.34%	3.394%
19	11.675	1422	1426	1433	rVB8	7130	11786	0.10%	0.012%
20	12.440	1546	1556	1563	rVB3	38647	74372	0.64%	0.074%
21	12.734	1599	1606	1611	rVV3	15901	29253	0.25%	0.029%
22	13.457	1724	1729	1734	rBV8	6211	13532	0.12%	0.013%
23	13.528	1736	1741	1747	rVB3	32317	54846	0.47%	0.054%
24	13.993	1814	1820	1826	rBV3	5624	13392	0.11%	0.013%
25	14.098	1831	1838	1852	rVV	4170211	5782067	49.57%	5.736%
26	14.193	1852	1854	1859	rVB6	7607	12259	0.11%	0.012%
27	14.387	1879	1887	1910	rBV	4798508	7072755	60.64%	7.016%
28	14.687	1931	1938	1944	rBV	3028766	4379891	37.55%	4.345%
29	14.745	1944	1948	1955	rVB	56841	84492	0.72%	0.084%
30	14.834	1959	1963	1967	rVB	13728	18749	0.16%	0.019%
31	14.892	1967	1973	1994	rBV	242615	520344	4.46%	0.516%
32	15.081	2001	2005	2009	rBV	27123	35229	0.30%	0.035%
33	15.322	2041	2046	2049	rBV7	9213	12040	0.10%	0.012%
34	15.416	2058	2062	2068	rVB5	8970	16714	0.14%	0.017%
35	15.681	2100	2107	2114	rBV	6682667	9269078	79.47%	9.195%
36	15.734	2114	2116	2121	rVV2	49547	78746	0.68%	0.078%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016791.D
 Acq On : 28 Aug 2023 14:14
 Operator : MA/JU
 Sample : 04134-12
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCHK6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

37	15.798	2121	2127	2143	rVV	1847409	2621870	22.48%	2.601%
38	15.916	2143	2147	2153	rVB2	27819	46158	0.40%	0.046%
39	16.257	2201	2205	2215	rVB5	12539	22403	0.19%	0.022%
40	17.081	2340	2345	2348	rBV6	12268	19941	0.17%	0.020%
41	17.116	2349	2351	2358	rVB8	13003	21092	0.18%	0.021%
42	17.245	2369	2373	2377	rBV4	7343	14054	0.12%	0.014%
43	17.451	2402	2408	2419	rBV	3675492	5249635	45.01%	5.207%
44	17.557	2419	2426	2436	rBV	7589165	10942790	93.82%	10.855%
45	17.875	2476	2480	2486	rVB2	20157	29503	0.25%	0.029%
46	18.028	2503	2506	2511	rBV7	10869	14075	0.12%	0.014%
47	18.081	2511	2515	2520	rVV7	16387	22955	0.20%	0.023%
48	18.292	2547	2551	2559	rBV2	55967	94060	0.81%	0.093%
49	19.357	2729	2732	2736	rVB2	92596	111233	0.95%	0.110%
50	19.428	2740	2744	2754	rVB2	80361	120750	1.04%	0.120%
51	19.522	2757	2760	2765	rBV2	48173	73381	0.63%	0.073%
52	19.786	2799	2805	2816	rBV	8951855	11663910	100.00%	11.570%
53	21.551	3100	3105	3112	rBV	3160634	4095924	35.12%	4.063%
54	23.951	3505	3513	3526	rVB2	4216803	8469384	72.61%	8.401%
55	24.121	3536	3542	3553	rVB	1772996	3649304	31.29%	3.620%




Sum of corrected areas: 100810275

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016791.D
Acq On : 28 Aug 2023 14:14
Operator : MA/JU
Sample : 04134-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHK6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

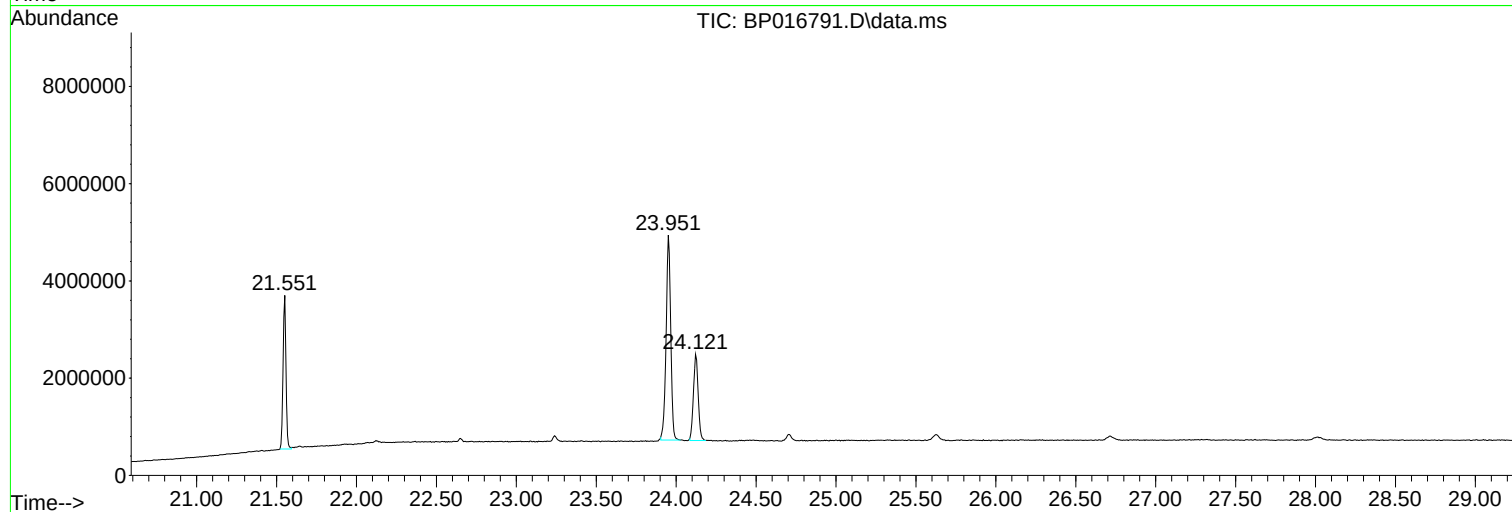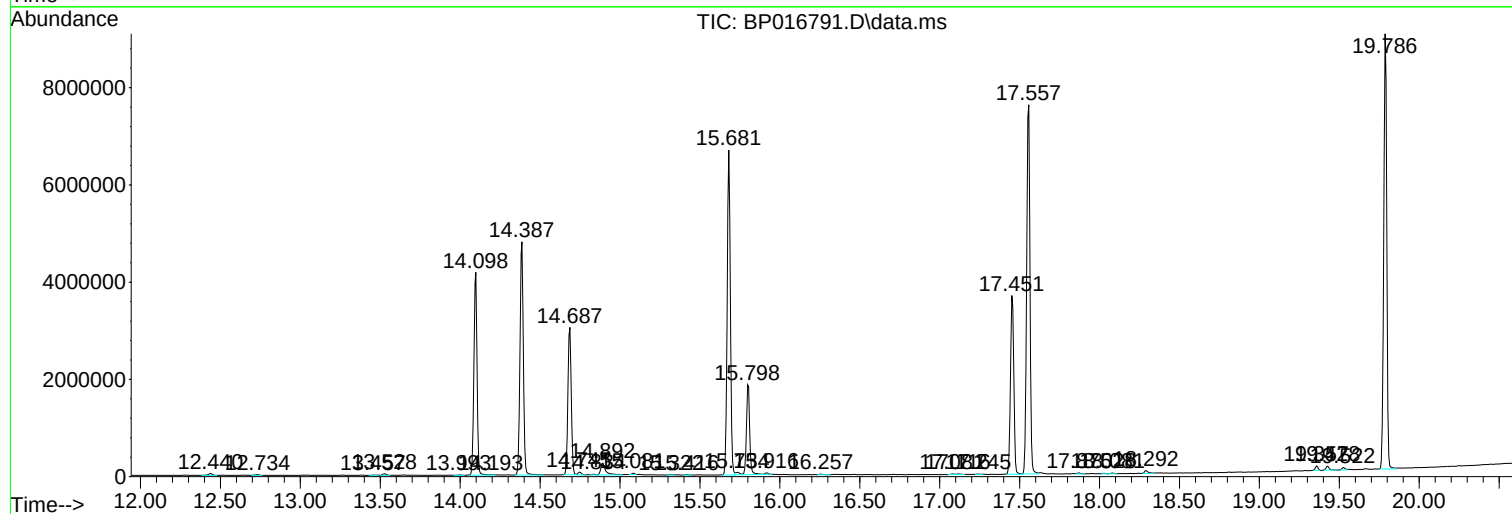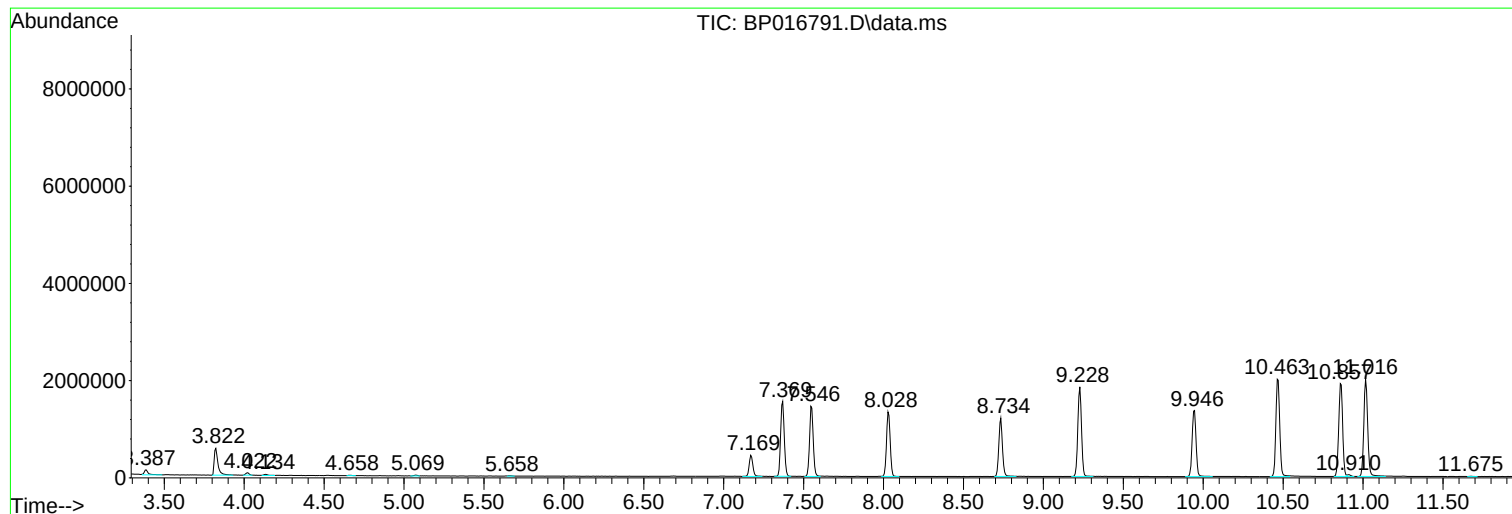

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016791.D
Acq On : 28 Aug 2023 14:14
Operator : MA/JU
Sample : 04134-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHK6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016791.D
Acq On : 28 Aug 2023 14:14
Operator : MA/JU
Sample : 04134-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHK6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
