

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016794.D
 Acq On : 28 Aug 2023 16:26
 Operator : MA/JU
 Sample : PB155078BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK078

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016794.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	12	16	29	rVB	142891	222734	2.10%	0.216%
2	3.817	86	90	113	rBV	1432904	2441966	23.01%	2.364%
3	4.134	140	144	150	rVB2	18516	28374	0.27%	0.027%
4	7.169	653	660	673	rBV	1827523	2845771	26.82%	2.755%
5	7.363	686	693	705	rVB	1482022	2287771	21.56%	2.215%
6	7.546	717	724	736	rBV	1772325	2760072	26.01%	2.672%
7	8.028	799	806	815	rBV	1283712	2000279	18.85%	1.936%
8	8.734	918	926	945	rBV	2127487	3542245	33.38%	3.429%
9	9.228	999	1010	1018	rBV	1709969	2787484	26.27%	2.698%
10	9.940	1121	1131	1145	rBV	1376106	2264419	21.34%	2.192%
11	10.463	1213	1220	1236	rBV	2081856	3540639	33.36%	3.428%
12	10.857	1279	1287	1298	rBV	1855297	3099437	29.21%	3.000%
13	11.016	1305	1314	1334	rBV	2164597	3707460	34.94%	3.589%
14	12.440	1548	1556	1561	rBV	35858	59547	0.56%	0.058%
15	13.534	1735	1742	1748	rBV	29348	48002	0.45%	0.046%
16	14.098	1831	1838	1852	rBV	3792305	5351946	50.43%	5.181%
17	14.387	1879	1887	1902	rBV	4594710	6652763	62.69%	6.440%
18	14.687	1931	1938	1954	rBV	3003670	4287438	40.40%	4.150%
19	14.887	1966	1972	1994	rBV	1402359	2537462	23.91%	2.456%
20	15.681	2100	2107	2122	rBV	5960031	8369473	78.87%	8.102%
21	15.804	2122	2128	2143	rVV	1484487	2136860	20.14%	2.069%
22	15.916	2143	2147	2155	rVB3	28177	50196	0.47%	0.049%
23	17.122	2348	2352	2359	rVB9	8751	12918	0.12%	0.013%
24	17.233	2369	2371	2379	rVB3	8437	13396	0.13%	0.013%
25	17.451	2402	2408	2419	rBV	3686089	5285306	49.80%	5.116%
26	17.557	2419	2426	2447	rVV	6479844	9264656	87.30%	8.969%
27	19.357	2728	2732	2738	rBV	80520	109454	1.03%	0.106%
28	19.427	2741	2744	2748	rVB	69451	81015	0.76%	0.078%
29	19.786	2799	2805	2816	rBV	8136987	10612029	100.00%	10.273%
30	21.551	3100	3105	3116	rBV	3757216	4996748	47.09%	4.837%
31	23.957	3506	3514	3525	rVB2	3647700	7800088	73.50%	7.551%
32	24.127	3536	3543	3552	rVB	1931569	4102836	38.66%	3.972%




Sum of corrected areas: 103300784

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016794.D
Acq On : 28 Aug 2023 16:26
Operator : MA/JU
Sample : PB155078BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK078

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

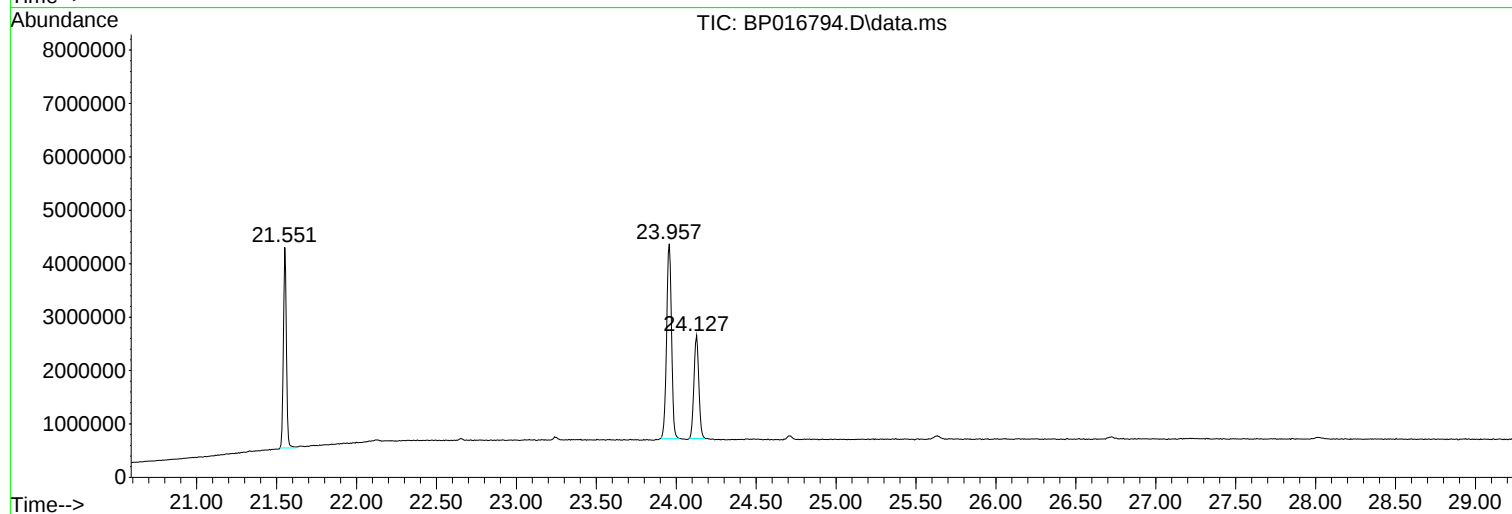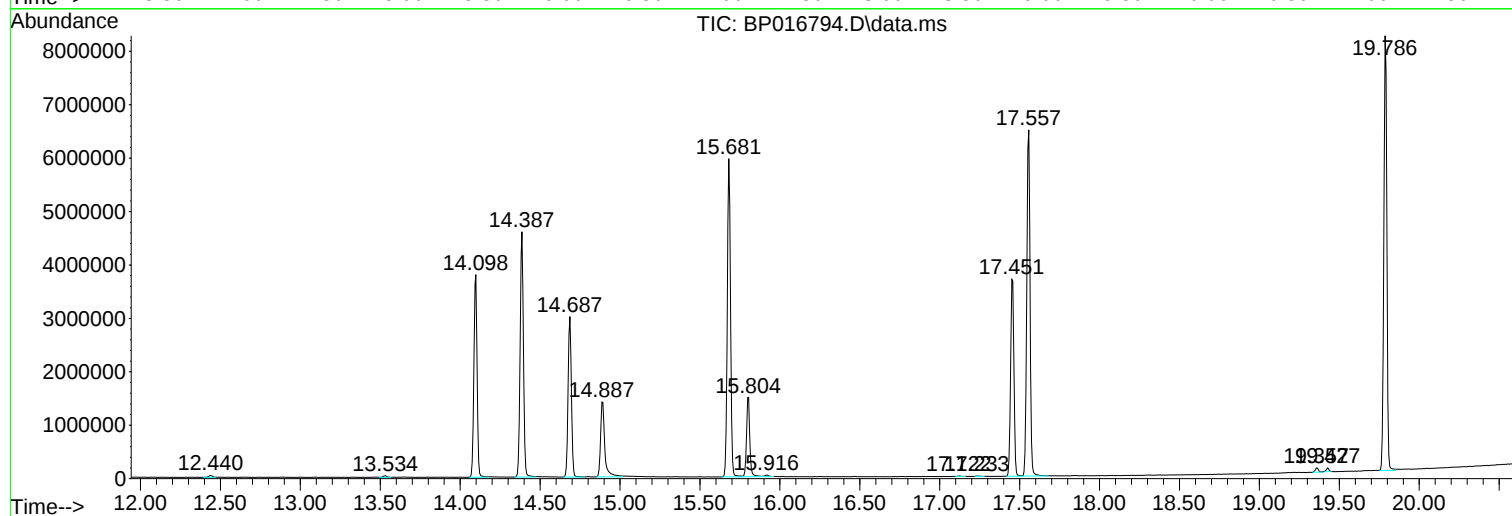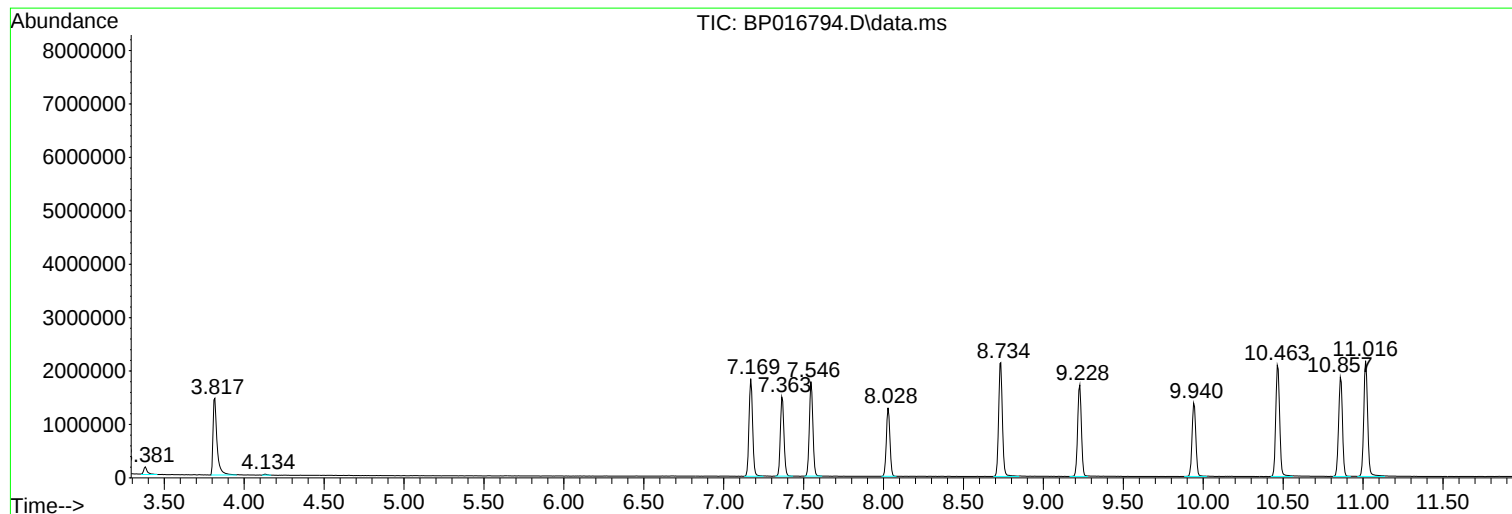

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016794.D
Acq On : 28 Aug 2023 16:26
Operator : MA/JU
Sample : PB155078BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK078

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016794.D
Acq On : 28 Aug 2023 16:26
Operator : MA/JU
Sample : PB155078BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK078

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc