

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016805.D
 Acq On : 28 Aug 2023 22:41
 Operator : MA/JU
 Sample : 04134-18
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCHI6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016805.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	12	16	25	rVB	101037	153535	1.16%	0.135%
2	3.822	87	91	106	rBV	549346	935375	7.07%	0.821%
3	4.016	120	124	132	rVB	47058	79927	0.60%	0.070%
4	4.134	140	144	149	rBV2	21293	31653	0.24%	0.028%
5	5.075	300	304	309	rVB	15524	22164	0.17%	0.019%
6	5.657	401	403	410	rVB5	9635	14602	0.11%	0.013%
7	7.169	654	660	675	rVB	436297	701886	5.30%	0.616%
8	7.369	686	694	704	rBV	1661934	2594089	19.60%	2.277%
9	7.545	717	724	737	rBV	1517311	2449817	18.51%	2.151%
10	8.028	800	806	817	rBV	1376798	2184485	16.51%	1.918%
11	8.734	918	926	935	rBV	1241432	2030564	15.35%	1.782%
12	8.898	946	954	961	rVB4	16085	37096	0.28%	0.033%
13	9.228	1001	1010	1019	rBV	1984436	3220745	24.34%	2.827%
14	9.457	1043	1049	1056	rVB3	17434	35391	0.27%	0.031%
15	9.939	1121	1131	1139	rBV	1519301	2528125	19.11%	2.219%
16	10.010	1139	1143	1146	rVV4	23923	44930	0.34%	0.039%
17	10.045	1146	1149	1155	rVB3	18514	27914	0.21%	0.025%
18	10.322	1191	1196	1201	rVB3	16980	27317	0.21%	0.024%
19	10.463	1213	1220	1234	rBV	2207247	3728946	28.18%	3.273%
20	10.857	1280	1287	1294	rBV	2052596	3352228	25.33%	2.943%
21	11.016	1306	1314	1330	rBV	2099713	3659064	27.65%	3.212%
22	11.228	1345	1350	1359	rVB6	49127	104923	0.79%	0.092%
23	11.457	1383	1389	1399	rVB7	18220	51333	0.39%	0.045%
24	11.675	1422	1426	1435	rVB3	12750	22589	0.17%	0.020%
25	11.869	1455	1459	1463	rBV6	9058	14463	0.11%	0.013%
26	11.933	1463	1470	1476	rVV9	12028	28795	0.22%	0.025%
27	12.198	1510	1515	1520	rVB5	10637	17835	0.13%	0.016%
28	12.269	1520	1527	1534	rBV	61831	108515	0.82%	0.095%
29	12.433	1546	1555	1562	rVB2	43949	87931	0.66%	0.077%
30	12.516	1562	1569	1573	rBV5	11979	21727	0.16%	0.019%
31	12.645	1582	1591	1596	rBV9	7362	18448	0.14%	0.016%
32	12.728	1596	1605	1614	rVB5	22098	55760	0.42%	0.049%
33	13.151	1672	1677	1683	rBV10	8668	22512	0.17%	0.020%
34	13.386	1712	1717	1720	rBV7	9312	16016	0.12%	0.014%
35	13.439	1720	1726	1735	rVV3	32307	65092	0.49%	0.057%
36	13.522	1735	1740	1750	rVB4	46839	87511	0.66%	0.077%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016805.D
 Acq On : 28 Aug 2023 22:41
 Operator : MA/JU
 Sample : 04134-18
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCHI6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

37	13.645	1757	1761	1766	rBV5	8335	14438	0.11%	0.013%
38	13.833	1785	1793	1795	rBV7	10122	23377	0.18%	0.021%
39	13.869	1795	1799	1802	rVV6	8938	15154	0.11%	0.013%
40	13.927	1805	1809	1813	rVV4	12906	21008	0.16%	0.018%
41	13.992	1816	1820	1826	rVB7	12123	22775	0.17%	0.020%
42	14.092	1831	1837	1848	rBV	4572735	6301531	47.62%	5.532%
43	14.227	1856	1860	1865	rVB6	11449	18453	0.14%	0.016%
44	14.380	1879	1886	1904	rBV	5149567	7812981	59.04%	6.858%
45	14.680	1927	1937	1944	rBV	3149167	4586661	34.66%	4.026%
46	14.745	1944	1948	1954	rVV	257609	369091	2.79%	0.324%
47	14.833	1958	1963	1967	rVV	68158	93402	0.71%	0.082%
48	14.886	1967	1972	1981	rVV	286612	525382	3.97%	0.461%
49	14.957	1981	1984	1993	rVB4	32801	65983	0.50%	0.058%
50	15.080	2000	2005	2009	rBV	66914	99657	0.75%	0.087%
51	15.122	2009	2012	2018	rVB	39197	62510	0.47%	0.055%
52	15.216	2024	2028	2032	rVB6	12907	16586	0.13%	0.015%
53	15.304	2037	2043	2048	rBV10	9464	19757	0.15%	0.017%
54	15.410	2055	2061	2071	rBV	144504	229596	1.74%	0.202%
55	15.492	2071	2075	2079	rVB5	11558	18459	0.14%	0.016%
56	15.622	2092	2097	2099	rBV	42188	61053	0.46%	0.054%
57	15.680	2100	2107	2113	rVV	7017369	10108738	76.39%	8.874%
58	15.733	2113	2116	2121	rVV	93516	152445	1.15%	0.134%
59	15.798	2121	2127	2143	rVV	2136547	3033122	22.92%	2.663%
60	15.916	2143	2147	2157	rVB3	34333	71968	0.54%	0.063%
61	16.033	2162	2167	2175	rVB5	15255	38443	0.29%	0.034%
62	16.180	2188	2192	2195	rBV4	10496	15464	0.12%	0.014%
63	16.416	2222	2232	2239	rBV2	94427	202214	1.53%	0.178%
64	16.621	2264	2267	2272	rVB6	12389	19217	0.15%	0.017%
65	16.710	2272	2282	2286	rBV5	22526	52322	0.40%	0.046%
66	17.068	2339	2343	2347	rBV3	50955	81836	0.62%	0.072%
67	17.233	2366	2371	2375	rBV3	15271	31573	0.24%	0.028%
68	17.451	2399	2408	2418	rBV	3973881	5688805	42.99%	4.994%
69	17.551	2418	2425	2440	rVB	8275004	11542406	87.23%	10.132%
70	17.692	2447	2449	2455	rVB7	11970	17355	0.13%	0.015%
71	17.792	2462	2466	2467	rBV4	15261	19480	0.15%	0.017%
72	17.863	2474	2478	2485	rVB	119252	171017	1.29%	0.150%
73	17.951	2489	2493	2499	rVB3	25106	37509	0.28%	0.033%
74	18.015	2500	2504	2510	rVB	21659	31226	0.24%	0.027%
75	18.286	2545	2550	2558	rBV2	181824	285039	2.15%	0.250%
76	18.433	2572	2575	2579	rBV3	18401	23642	0.18%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016805.D
 Acq On : 28 Aug 2023 22:41
 Operator : MA/JU
 Sample : 04134-18
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCHI6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M

Title : SVOA CALIBRATION

77	19.351	2727	2731	2736	rBV	108467	152543	1.15%	0.134%
78	19.421	2739	2743	2751	rVB	101544	156441	1.18%	0.137%
79	19.515	2756	2759	2767	rBV4	70862	119431	0.90%	0.105%
80	19.786	2799	2805	2820	rBV	9761763	13232578	100.00%	11.616%
81	21.198	3042	3045	3056	rVB5	159375	248389	1.88%	0.218%
82	21.545	3099	3104	3113	rBV	4047823	5121847	38.71%	4.496%
83	23.945	3503	3512	3522	rVB2	4682977	10032105	75.81%	8.806%
84	24.115	3534	3541	3549	rVB	2036923	4270087	32.27%	3.748%




Sum of corrected areas: 113918399

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016805.D
Acq On : 28 Aug 2023 22:41
Operator : MA/JU
Sample : 04134-18
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHI6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

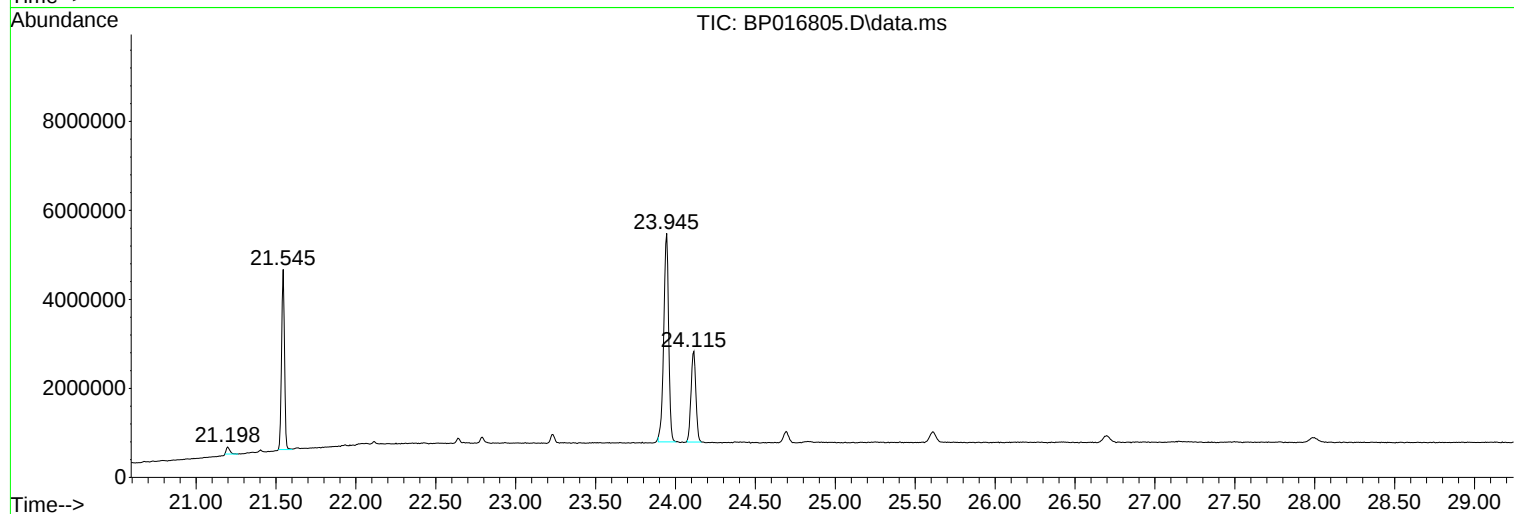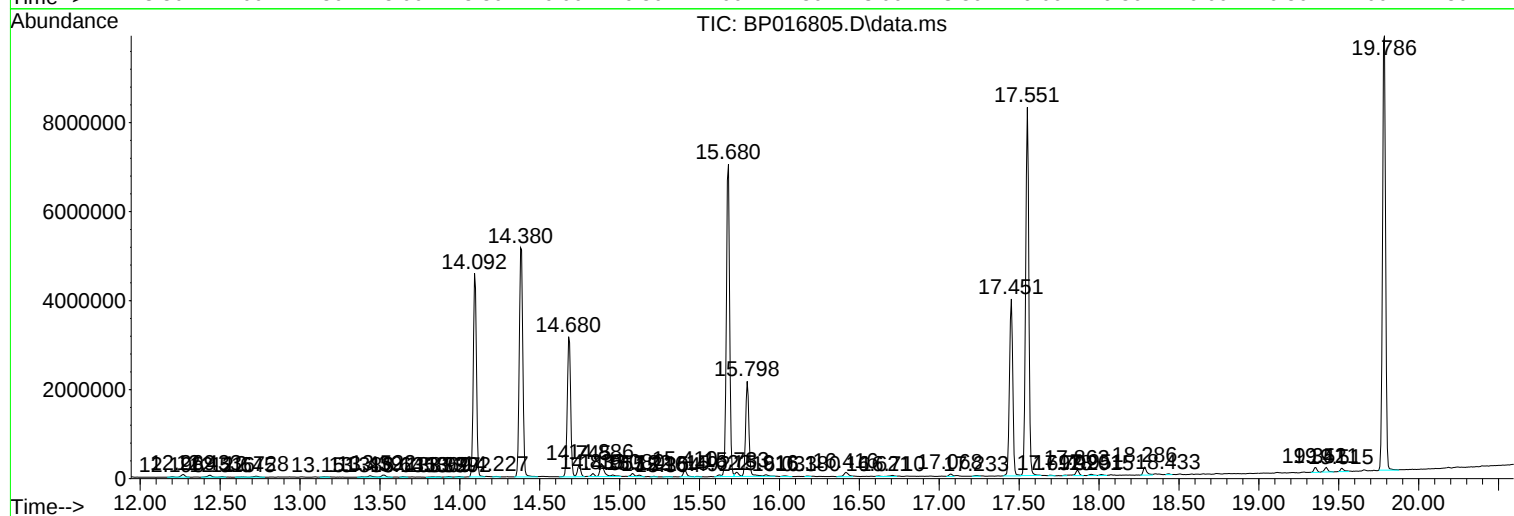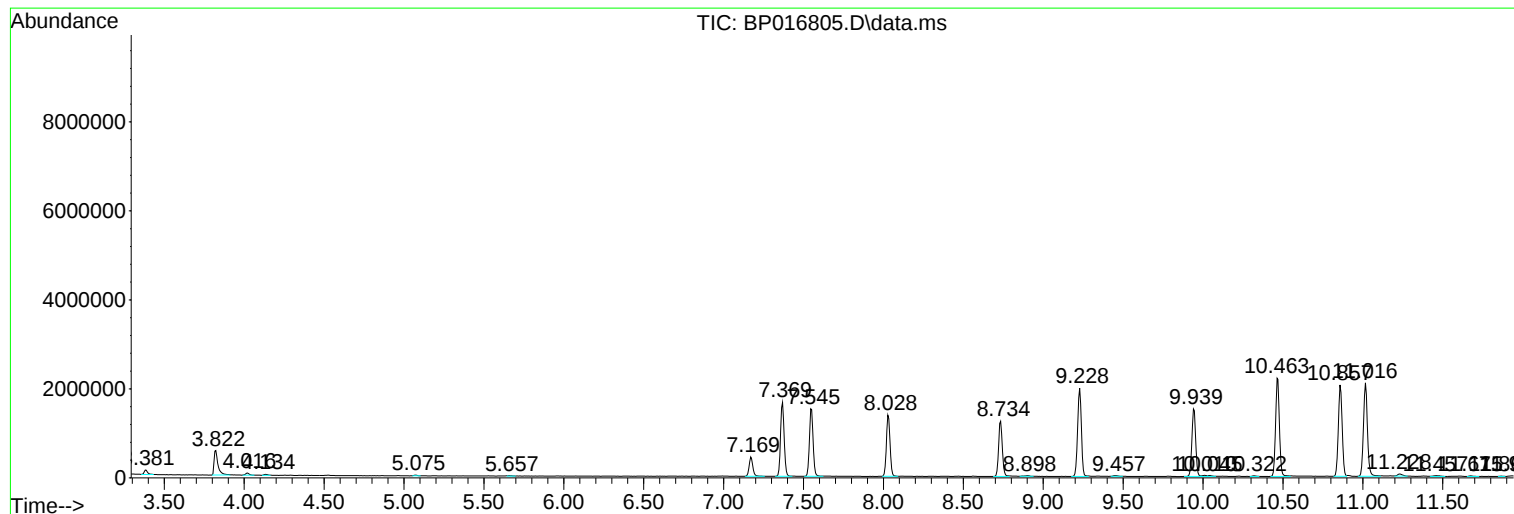

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016805.D
Acq On : 28 Aug 2023 22:41
Operator : MA/JU
Sample : 04134-18
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHI6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016805.D
Acq On : 28 Aug 2023 22:41
Operator : MA/JU
Sample : 04134-18
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHI6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc