

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016806.D
 Acq On : 28 Aug 2023 23:15
 Operator : MA/JU
 Sample : 04134-22
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCHI8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016806.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	13	16	23	rVB	73789	100506	0.82%	0.096%
2	3.822	87	91	113	rVB	379219	647956	5.26%	0.619%
3	4.022	120	125	132	rVB	35877	61397	0.50%	0.059%
4	4.134	140	144	148	rBV3	17354	24987	0.20%	0.024%
5	5.075	300	304	308	rBV2	10240	14517	0.12%	0.014%
6	7.169	654	660	671	rVB	316795	514238	4.18%	0.491%
7	7.369	683	694	706	rBV	1447772	2304066	18.71%	2.201%
8	7.546	717	724	736	rBV	1269176	2052373	16.67%	1.960%
9	7.634	736	739	748	rVB7	7535	17866	0.15%	0.017%
10	8.028	799	806	817	rVB	1450892	2310355	18.76%	2.207%
11	8.381	859	866	873	rBV6	14409	29267	0.24%	0.028%
12	8.734	918	926	937	rBV	1018531	1654283	13.44%	1.580%
13	9.228	1002	1010	1023	rBV	1771316	2867010	23.29%	2.739%
14	9.446	1043	1047	1056	rVB2	24802	40469	0.33%	0.039%
15	9.940	1121	1131	1146	rBV	1331032	2239401	18.19%	2.139%
16	10.463	1212	1220	1240	rBV	1887560	3275362	26.60%	3.129%
17	10.857	1279	1287	1305	rBV	2141616	3590911	29.17%	3.430%
18	11.016	1305	1314	1330	rBV	1497671	2584283	20.99%	2.469%
19	11.228	1347	1350	1360	rVB8	10917	23657	0.19%	0.023%
20	11.945	1466	1472	1477	rVB	32329	49134	0.40%	0.047%
21	12.439	1550	1556	1563	rVB	39673	65558	0.53%	0.063%
22	13.322	1703	1706	1713	rVB9	7610	13453	0.11%	0.013%
23	13.528	1734	1741	1747	rVB3	22572	38936	0.32%	0.037%
24	13.651	1757	1762	1767	rVB7	6655	13811	0.11%	0.013%
25	13.934	1804	1810	1816	rBV2	11166	20820	0.17%	0.020%
26	14.092	1830	1837	1851	rBV	4218660	5877324	47.74%	5.614%
27	14.381	1879	1886	1901	rBV2	4687154	7089058	57.58%	6.771%
28	14.681	1930	1937	1948	rBV	3313923	4860855	39.48%	4.643%
29	14.892	1966	1973	1988	rBV	187749	417295	3.39%	0.399%
30	15.492	2070	2075	2079	rVB7	9250	13284	0.11%	0.013%
31	15.680	2099	2107	2113	rBV	6296313	9090182	73.83%	8.683%
32	15.733	2113	2116	2121	rVV3	55765	105190	0.85%	0.100%
33	15.798	2121	2127	2143	rVV	1983692	2715938	22.06%	2.594%
34	15.916	2143	2147	2154	rVB	34023	57378	0.47%	0.055%
35	16.257	2201	2205	2212	rVB9	16735	25537	0.21%	0.024%
36	16.469	2236	2241	2246	rBV	66740	90879	0.74%	0.087%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016806.D
 Acq On : 28 Aug 2023 23:15
 Operator : MA/JU
 Sample : 04134-22
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCHI8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

37	17.010	2329	2333	2339	rBV3	26845	35580	0.29%	0.034%
38	17.075	2340	2344	2348	rBV2	29346	42677	0.35%	0.041%
39	17.233	2369	2371	2377	rVB4	12201	18387	0.15%	0.018%
40	17.451	2401	2408	2417	rBV	4341237	6007666	48.79%	5.739%
41	17.551	2419	2425	2437	rVV	7467171	10460209	84.96%	9.992%
42	18.286	2546	2550	2561	rBV	193522	319095	2.59%	0.305%
43	19.357	2728	2732	2736	rBV2	100127	136812	1.11%	0.131%
44	19.421	2740	2743	2748	rVB	88999	117695	0.96%	0.112%
45	19.521	2756	2760	2767	rBV	131888	179151	1.46%	0.171%
46	19.786	2799	2805	2818	rBV	9372961	12312100	100.00%	11.760%
47	21.545	3099	3104	3114	rBV	4361629	5690790	46.22%	5.436%
48	23.945	3504	3512	3525	rVB2	4563696	9626672	78.19%	9.195%
49	24.115	3534	3541	3556	rVB	2244974	4845936	39.36%	4.629%




Sum of corrected areas: 104690306

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016806.D
Acq On : 28 Aug 2023 23:15
Operator : MA/JU
Sample : 04134-22
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHI8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

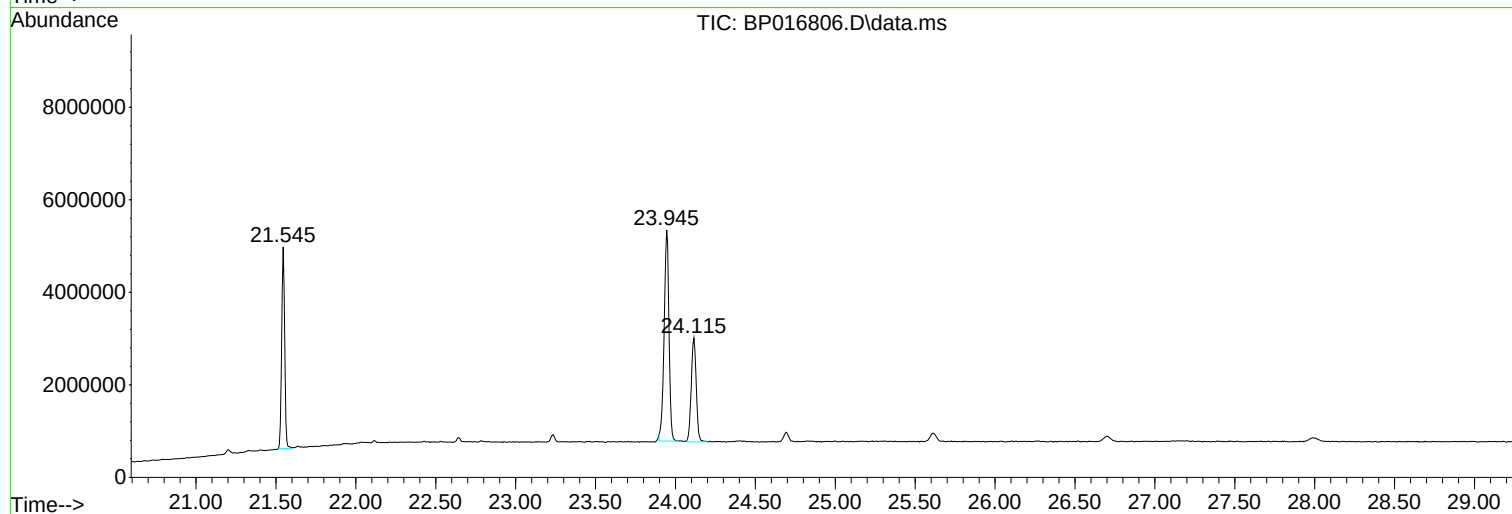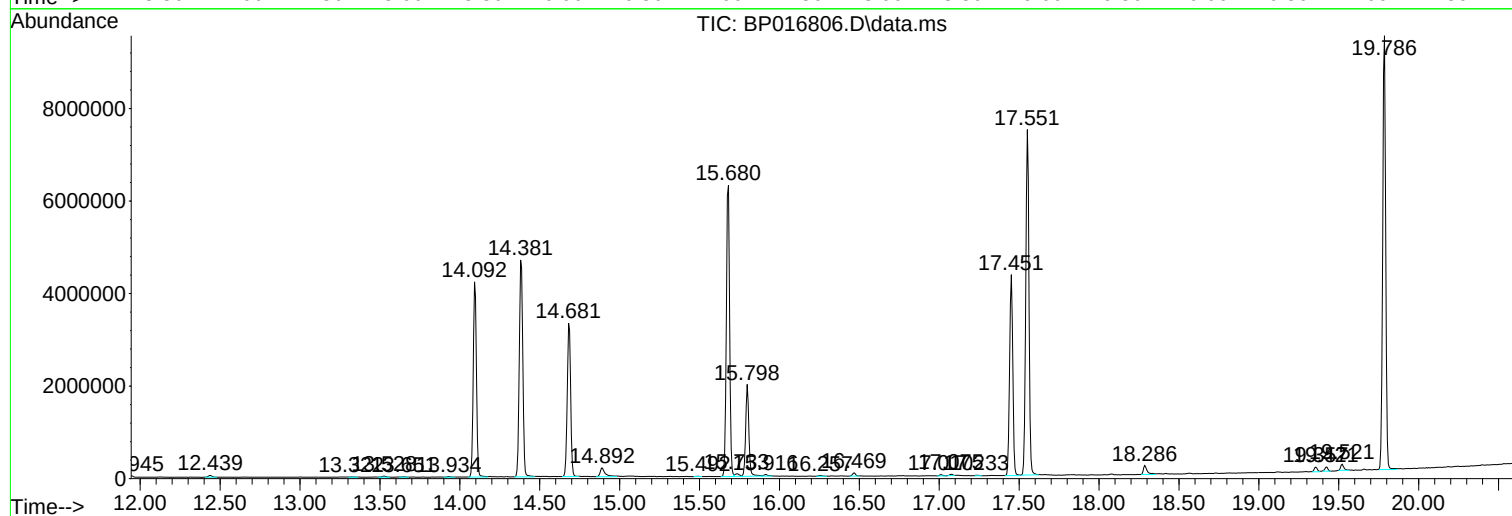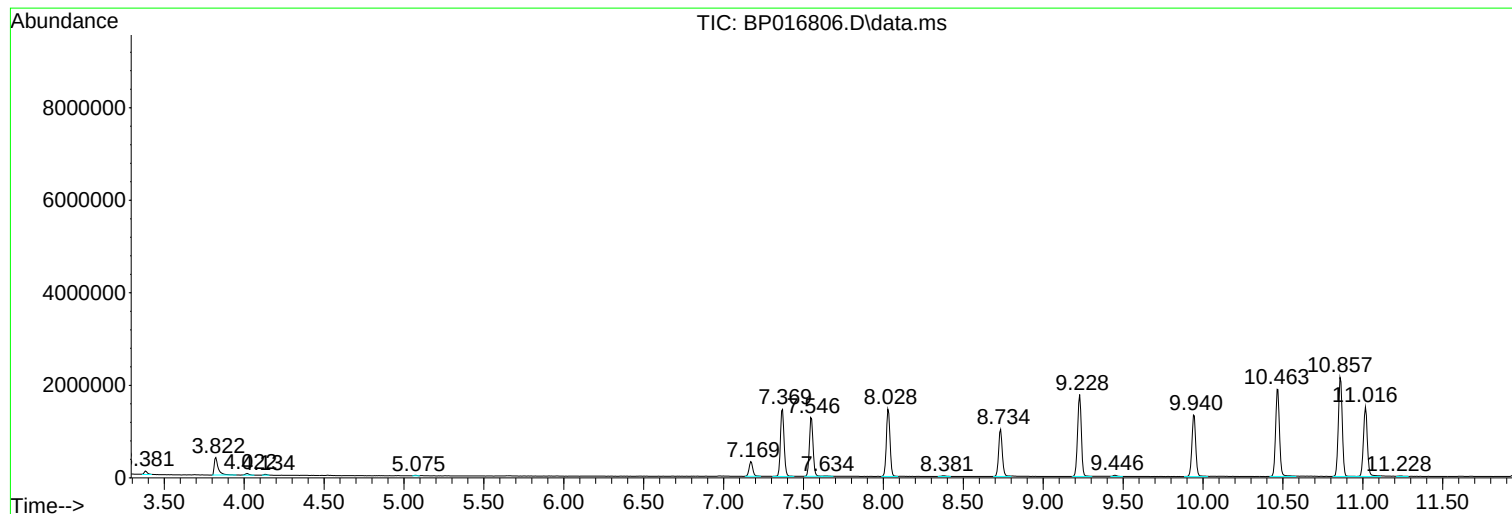

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016806.D
Acq On : 28 Aug 2023 23:15
Operator : MA/JU
Sample : 04134-22
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHI8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016806.D
Acq On : 28 Aug 2023 23:15
Operator : MA/JU
Sample : 04134-22
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHI8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc