

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016814.D
 Acq On : 29 Aug 2023 04:19
 Operator : MA/JU
 Sample : PB155098BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK098

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016814.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	12	16	27	rVB	142608	221969	1.94%	0.202%
2	3.817	85	90	109	rBV	1506046	2583659	22.58%	2.357%
3	4.134	140	144	150	rVB	17665	27270	0.24%	0.025%
4	7.169	653	660	678	rBV	1980619	3070416	26.83%	2.801%
5	7.363	684	693	703	rBV	1543517	2416926	21.12%	2.205%
6	7.546	717	724	736	rBV	1901507	2932015	25.62%	2.675%
7	8.028	798	806	816	rBV	1237882	1919309	16.77%	1.751%
8	8.728	918	925	942	rBV	2338185	3810759	33.30%	3.476%
9	9.222	1002	1009	1023	rBV	1806116	2991820	26.14%	2.729%
10	9.940	1122	1131	1143	rBV	1529889	2439137	21.31%	2.225%
11	10.463	1212	1220	1237	rBV	2282646	3821325	33.39%	3.486%
12	10.857	1278	1287	1295	rBV	1832464	3013995	26.34%	2.749%
13	11.016	1305	1314	1329	rBV	2302354	3949836	34.52%	3.603%
14	12.434	1549	1555	1562	rBV	39564	68947	0.60%	0.063%
15	13.528	1735	1741	1746	rBV	38640	61590	0.54%	0.056%
16	14.093	1830	1837	1851	rBV	4306679	5692693	49.75%	5.193%
17	14.381	1879	1886	1902	rBV	4909404	7115122	62.18%	6.491%
18	14.681	1930	1937	1949	rBV	2856019	4144969	36.22%	3.781%
19	14.887	1964	1972	1995	rBV	1645604	2863227	25.02%	2.612%
20	15.675	2099	2106	2121	rBV	6192143	8911268	77.87%	8.129%
21	15.798	2121	2127	2142	rVV	1701187	2358172	20.61%	2.151%
22	15.916	2143	2147	2156	rVB2	30312	56923	0.50%	0.052%
23	17.116	2347	2351	2354	rBV6	10156	12761	0.11%	0.012%
24	17.239	2367	2372	2377	rBV5	8671	16348	0.14%	0.015%
25	17.451	2401	2408	2417	rBV	3573906	5080524	44.40%	4.635%
26	17.551	2418	2425	2444	rVV	7213427	9901748	86.53%	9.033%
27	19.351	2727	2731	2736	rBV2	86375	123086	1.08%	0.112%
28	19.422	2740	2743	2748	rVB	70667	92412	0.81%	0.084%
29	19.780	2798	2804	2815	rBV	8863751	11443669	100.00%	10.439%
30	21.545	3099	3104	3114	rBV	3813642	4926554	43.05%	4.494%
31	23.945	3503	3512	3528	rVB2	4339858	9281055	81.10%	8.466%
32	24.116	3534	3541	3551	rVB	1960345	4271698	37.33%	3.897%




Sum of corrected areas: 109621202

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016814.D
Acq On : 29 Aug 2023 04:19
Operator : MA/JU
Sample : PB155098BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK098

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

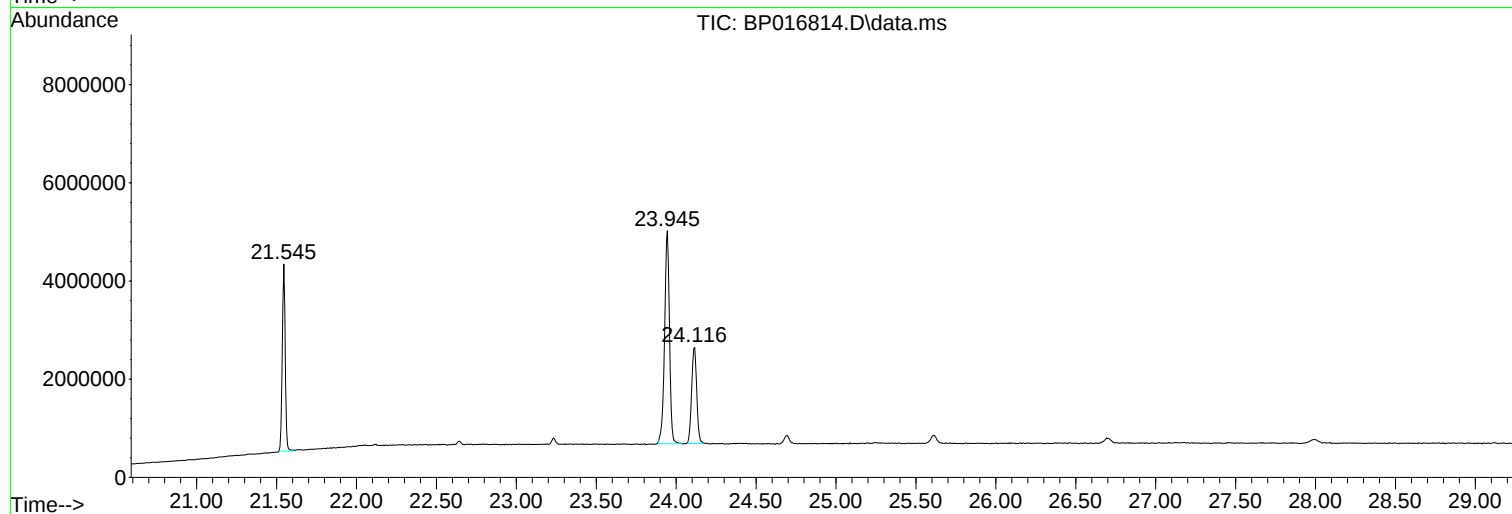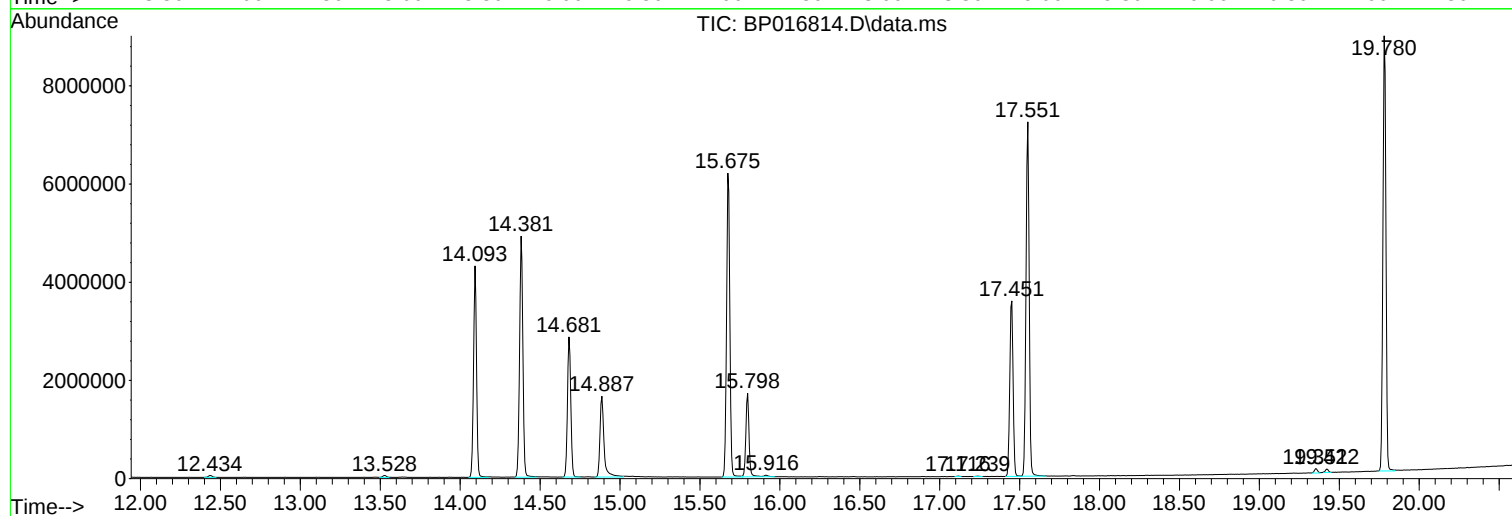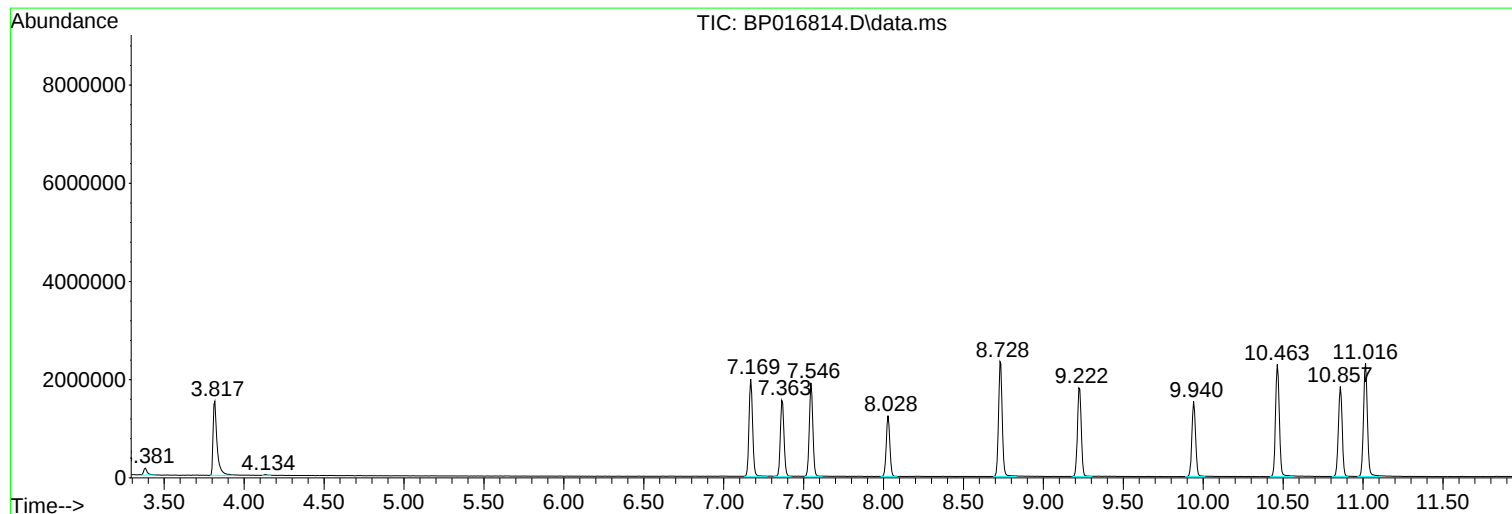

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016814.D
Acq On : 29 Aug 2023 04:19
Operator : MA/JU
Sample : PB155098BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK098

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016814.D
Acq On : 29 Aug 2023 04:19
Operator : MA/JU
Sample : PB155098BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK098

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc