

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016818.D
 Acq On : 29 Aug 2023 06:34
 Operator : MA/JU
 Sample : 04134-19
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCHI7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016818.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	13	16	28	rVB	124180	187825	1.37%	0.144%
2	3.817	87	90	106	rBV	727557	1162771	8.47%	0.891%
3	4.017	119	124	130	rVB	61042	93583	0.68%	0.072%
4	4.134	140	144	149	rVB	27280	36835	0.27%	0.028%
5	4.522	207	210	214	rVB3	10763	15377	0.11%	0.012%
6	5.069	299	303	308	rBV	19236	24463	0.18%	0.019%
7	5.658	399	403	409	rVB4	9150	15779	0.11%	0.012%
8	7.169	654	660	671	rBV	539937	837491	6.10%	0.642%
9	7.363	686	693	703	rBV	2019750	3138063	22.85%	2.404%
10	7.546	717	724	734	rBV	1903735	2953027	21.50%	2.262%
11	8.028	799	806	818	rBV	1881495	2950822	21.49%	2.261%
12	8.728	918	925	938	rBV	1512568	2477296	18.04%	1.898%
13	9.228	1002	1010	1022	rBV	2346372	3893412	28.35%	2.983%
14	9.446	1042	1047	1055	rVB2	25080	37807	0.28%	0.029%
15	9.940	1123	1131	1148	rBV	1936690	3127776	22.78%	2.396%
16	10.463	1212	1220	1235	rBV	2707273	4525631	32.96%	3.467%
17	10.857	1277	1287	1295	rBV	2766367	4531606	33.00%	3.472%
18	11.016	1304	1314	1333	rBV	2631931	4497744	32.75%	3.446%
19	11.940	1466	1471	1477	rVB	47259	70075	0.51%	0.054%
20	12.434	1547	1555	1561	rBV	51543	88545	0.64%	0.068%
21	12.734	1600	1606	1610	rVB7	8413	15937	0.12%	0.012%
22	13.434	1722	1725	1730	rBV3	8918	13754	0.10%	0.011%
23	13.522	1734	1740	1747	rVV3	58372	104073	0.76%	0.080%
24	14.092	1830	1837	1849	rBV	5861352	7911434	57.61%	6.061%
25	14.181	1849	1852	1857	rVB6	8666	17193	0.13%	0.013%
26	14.381	1879	1886	1898	rBV	6514151	9270736	67.51%	7.102%
27	14.681	1930	1937	1945	rBV	4131428	6062918	44.15%	4.645%
28	14.745	1945	1948	1954	rVB	31952	47210	0.34%	0.036%
29	14.887	1966	1972	1991	rBV	324494	642832	4.68%	0.492%
30	15.081	2000	2005	2008	rBV	44738	61183	0.45%	0.047%
31	15.316	2041	2045	2048	rBV6	9953	14045	0.10%	0.011%
32	15.675	2099	2106	2113	rBV	8175770	12007410	87.44%	9.199%
33	15.734	2113	2116	2121	rVV	71887	129010	0.94%	0.099%
34	15.798	2121	2127	2141	rVV	2620807	3631273	26.44%	2.782%
35	15.916	2143	2147	2156	rVB	40740	79749	0.58%	0.061%
36	16.457	2237	2239	2245	rVB5	9354	14510	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016818.D
 Acq On : 29 Aug 2023 06:34
 Operator : MA/JU
 Sample : 04134-19
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCHI7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

37	17.116	2347	2351	2356	rVB6	13864	20684	0.15%	0.016%
38	17.233	2367	2371	2375	rBV2	13117	19200	0.14%	0.015%
39	17.451	2401	2408	2418	rBV	5063559	7095217	51.67%	5.436%
40	17.551	2418	2425	2441	rVV	9483663	13152912	95.78%	10.077%
41	17.863	2475	2478	2484	rVB	40187	58926	0.43%	0.045%
42	18.075	2511	2514	2519	rVB5	29044	33415	0.24%	0.026%
43	18.281	2545	2549	2557	rBV2	125701	191410	1.39%	0.147%
44	19.351	2727	2731	2737	rBV2	113991	154144	1.12%	0.118%
45	19.422	2739	2743	2747	rVB	97322	130973	0.95%	0.100%
46	19.516	2756	2759	2767	rBV2	77845	117145	0.85%	0.090%
47	19.780	2798	2804	2814	rBV	10486584	13732039	100.00%	10.520%
48	21.545	3099	3104	3113	rBV	4237863	5381515	39.19%	4.123%
49	23.945	3503	3512	3525	rVB2	5071324	10651530	77.57%	8.160%
50	24.115	3534	3541	3556	rVB	2359087	5100096	37.14%	3.907%




Sum of corrected areas: 130528401

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016818.D
Acq On : 29 Aug 2023 06:34
Operator : MA/JU
Sample : 04134-19
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHI7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

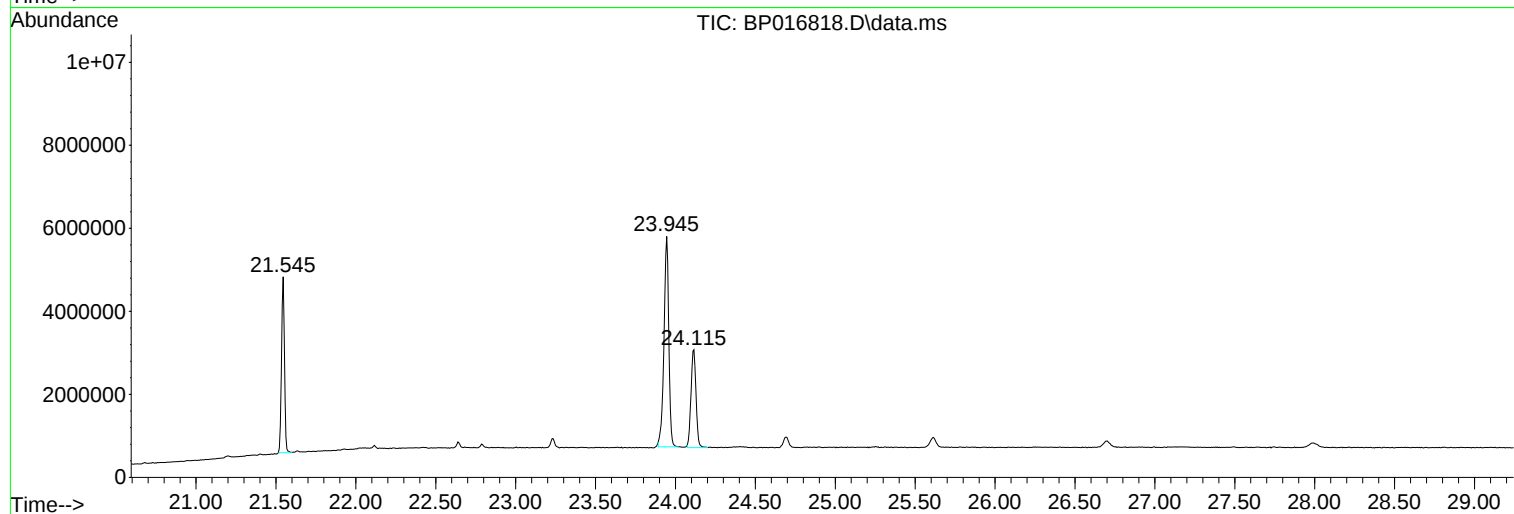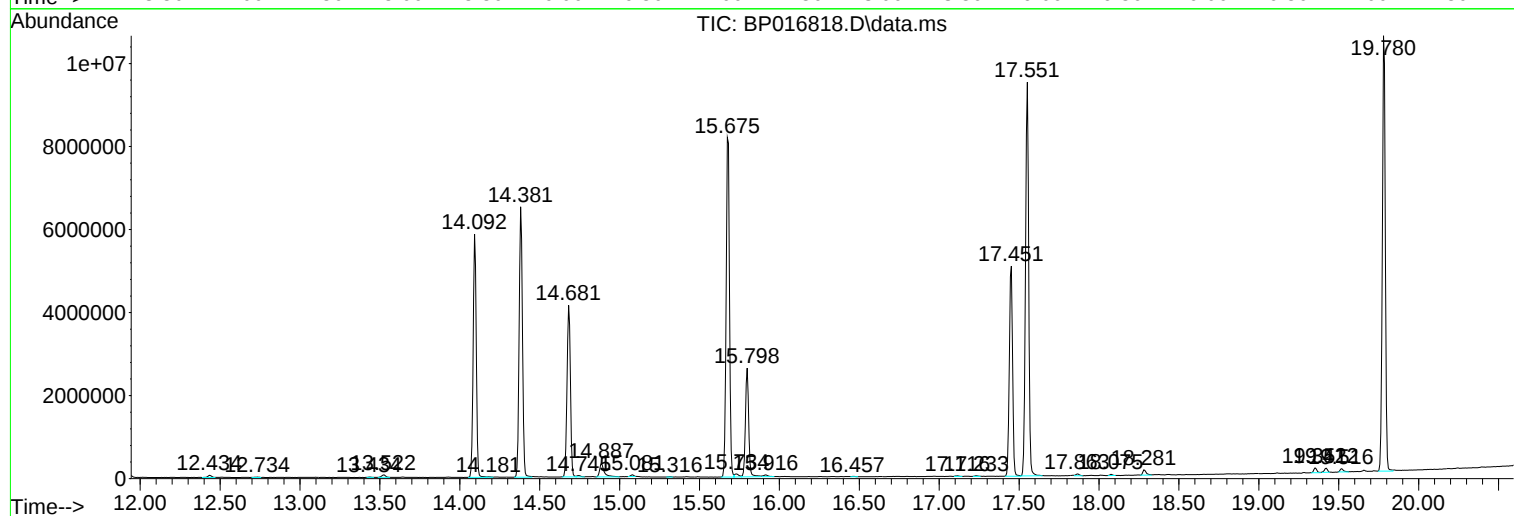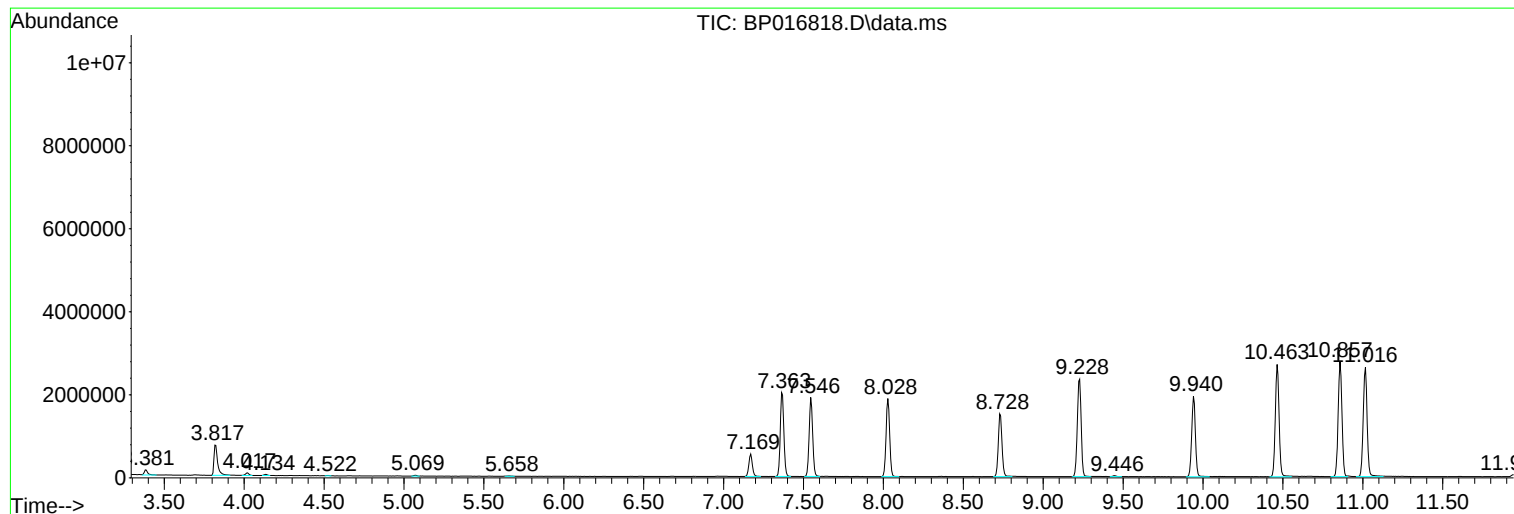

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016818.D
Acq On : 29 Aug 2023 06:34
Operator : MA/JU
Sample : 04134-19
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHI7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016818.D
Acq On : 29 Aug 2023 06:34
Operator : MA/JU
Sample : 04134-19
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHI7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------