

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016823.D
 Acq On : 29 Aug 2023 09:23
 Operator : MA/JU
 Sample : 04123-19
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH8R9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016823.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	5	8	13	rBV	57035	75085	0.25%	0.046%
2	3.381	13	16	21	rVV	128127	147790	0.49%	0.090%
3	3.817	87	90	109	rBV	662959	1045815	3.43%	0.640%
4	4.017	120	124	135	rVB	64695	102069	0.34%	0.062%
5	4.134	140	144	148	rBV	27332	36347	0.12%	0.022%
6	4.664	227	234	253	rVB	19061323	30450187	100.00%	18.641%
7	7.169	653	660	675	rVB	640680	996666	3.27%	0.610%
8	7.363	686	693	704	rBV	2209380	3478787	11.42%	2.130%
9	7.546	717	724	736	rBV	2130226	3346495	10.99%	2.049%
10	8.028	797	806	816	rBV	1793545	2803646	9.21%	1.716%
11	8.728	917	925	944	rBV	1714312	2820319	9.26%	1.727%
12	9.228	1000	1010	1021	rBV	2625764	4320024	14.19%	2.645%
13	9.940	1123	1131	1151	rBV	2135471	3434609	11.28%	2.103%
14	10.463	1211	1220	1236	rBV	3057338	4999040	16.42%	3.060%
15	10.857	1279	1287	1295	rBV	2607566	4273670	14.03%	2.616%
16	11.016	1306	1314	1332	rBV	2833789	4783342	15.71%	2.928%
17	12.434	1549	1555	1561	rVB2	56602	89495	0.29%	0.055%
18	13.528	1735	1741	1746	rBV	49894	81493	0.27%	0.050%
19	14.092	1830	1837	1849	rBV	5812674	7966600	26.16%	4.877%
20	14.381	1878	1886	1902	rBV2	6905721	9939766	32.64%	6.085%
21	14.592	1917	1922	1927	rVB	27632	40159	0.13%	0.025%
22	14.681	1930	1937	1946	rBV	3976093	5699039	18.72%	3.489%
23	14.887	1966	1972	1987	rBV	347149	680835	2.24%	0.417%
24	15.681	2099	2107	2120	rBV	8333570	12331187	40.50%	7.549%
25	15.798	2121	2127	2142	rVV	2583657	3630837	11.92%	2.223%
26	15.916	2142	2147	2156	rVB	42402	81302	0.27%	0.050%
27	17.451	2401	2408	2418	rBV	4700848	6659514	21.87%	4.077%
28	17.551	2418	2425	2443	rVV2	9333710	13252362	43.52%	8.113%
29	18.286	2546	2550	2559	rBV	160243	261747	0.86%	0.160%
30	19.351	2728	2731	2736	rBV2	108892	138660	0.46%	0.085%
31	19.422	2739	2743	2747	rVB	101721	138107	0.45%	0.085%
32	19.522	2756	2760	2765	rBV	112106	157133	0.52%	0.096%
33	19.786	2799	2805	2815	rBV	10682827	14040373	46.11%	8.595%
34	21.545	3099	3104	3115	rBV	3959798	5227959	17.17%	3.201%
35	23.945	3503	3512	3528	rVB2	5081657	11007712	36.15%	6.739%
36	24.115	3534	3541	3552	rVB	2303381	4808567	15.79%	2.944%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016823.D
Acq On : 29 Aug 2023 09:23
Operator : MA/JU
Sample : 04123-19
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH8R9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 163346738

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016823.D
Acq On : 29 Aug 2023 09:23
Operator : MA/JU
Sample : 04123-19
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH8R9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

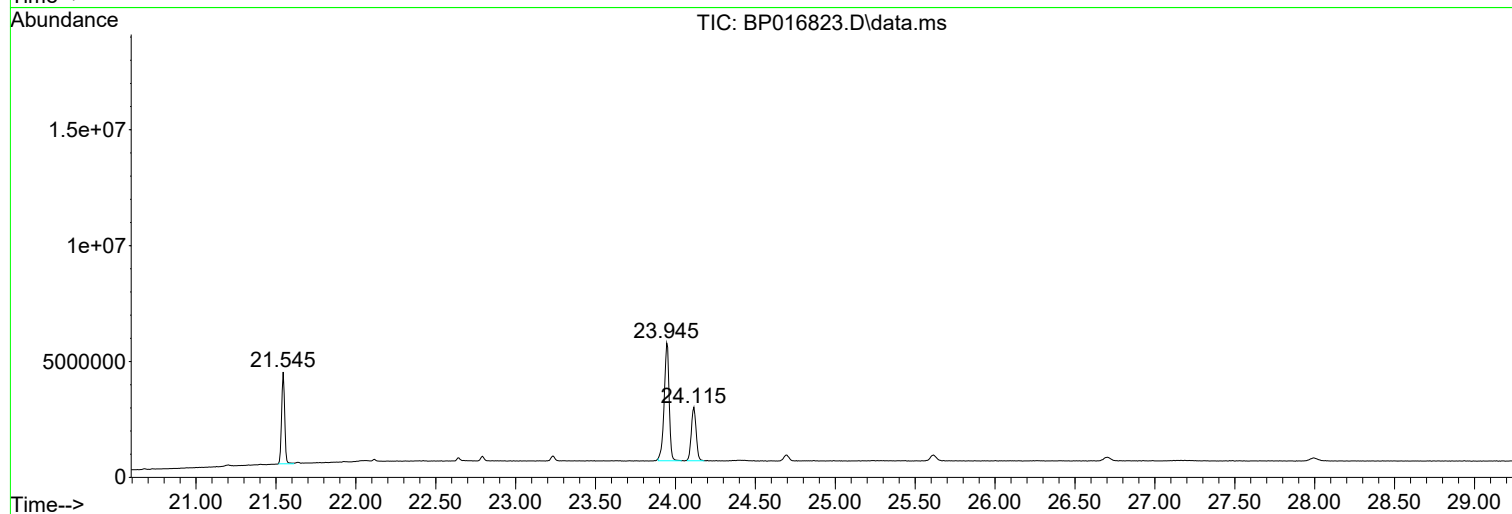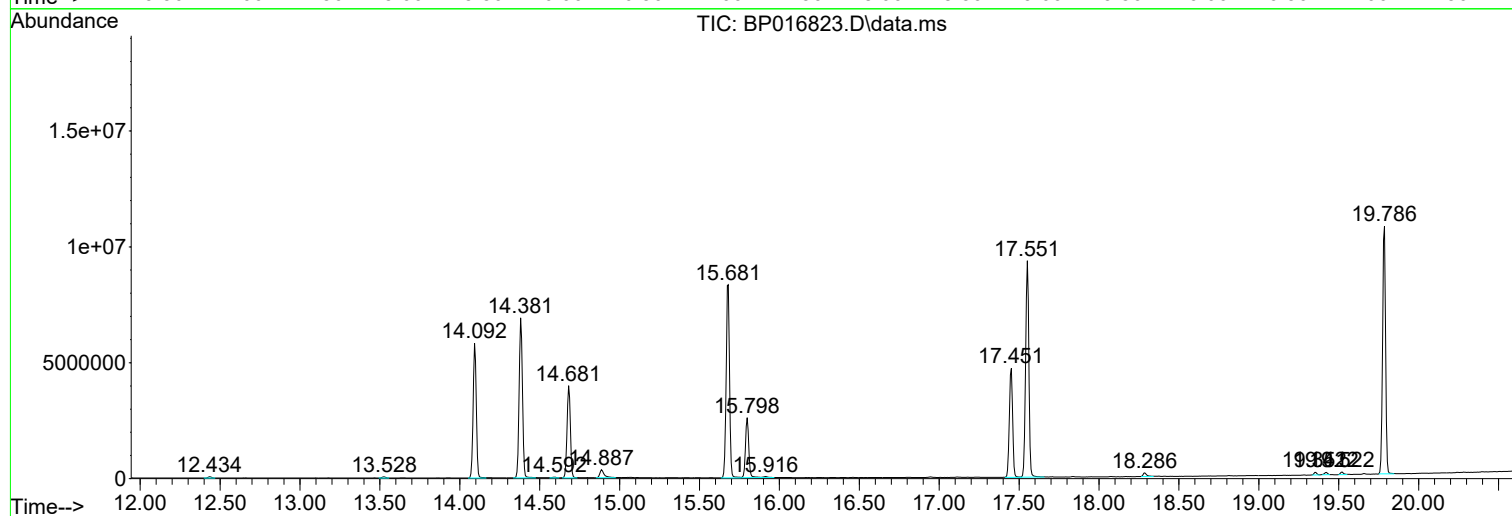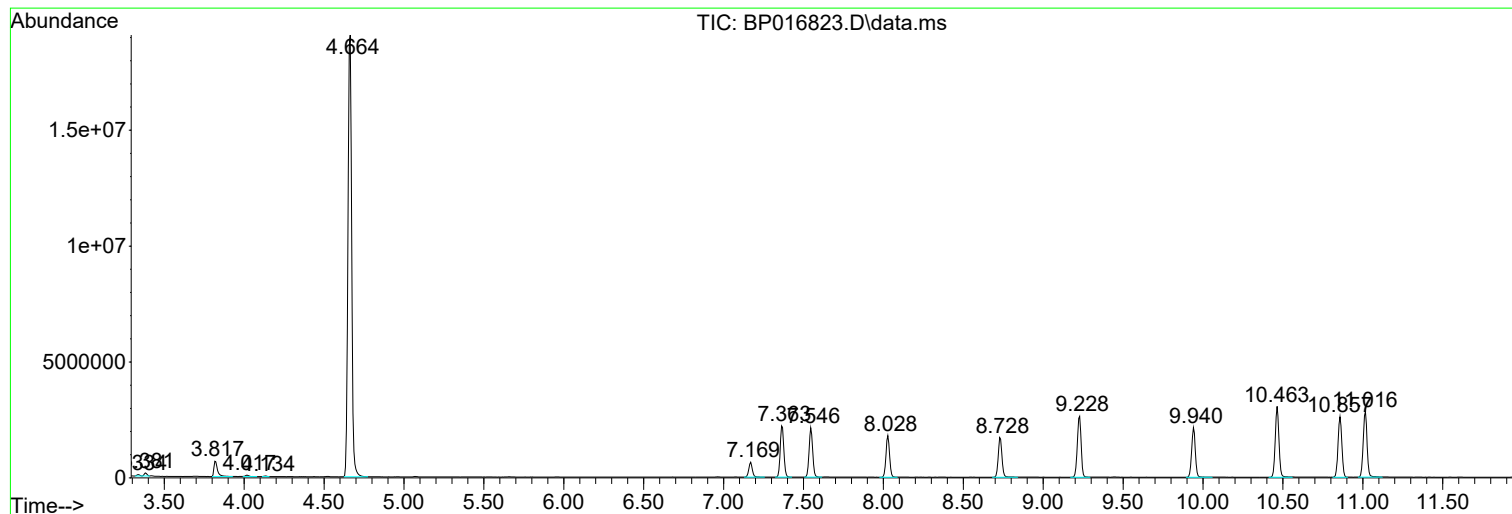

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016823.D
Acq On : 29 Aug 2023 09:23
Operator : MA/JU
Sample : 04123-19
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH8R9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.664	217.22 ng/ul	30450200	1,4-Dichlorobenzene-d4	8.028

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	94
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	38

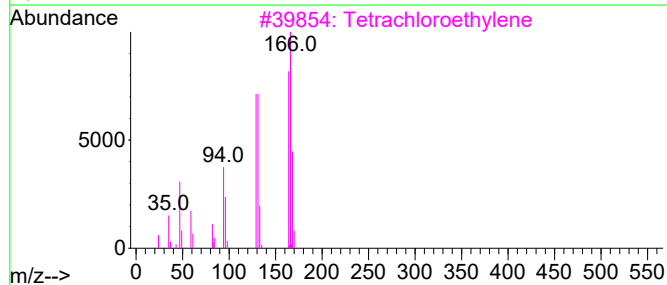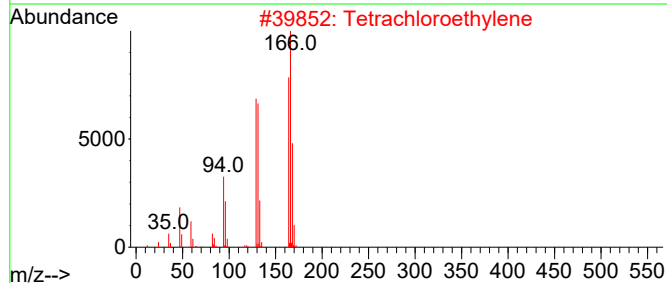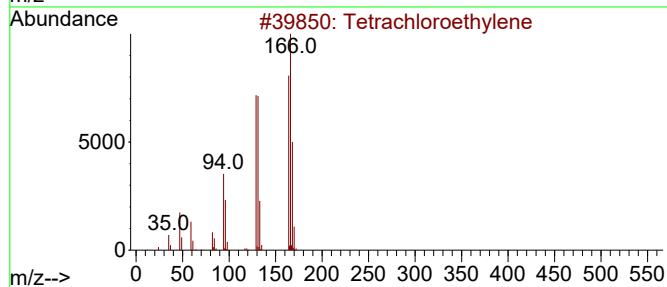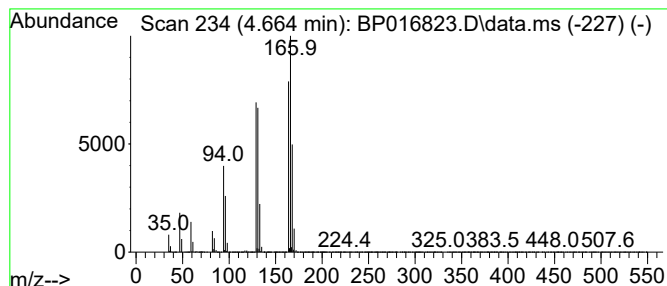

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016823.D
Acq On : 29 Aug 2023 09:23
Operator : MA/JU
Sample : 04123-19
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH8R9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.664	217.2	ng/ul	30450200	1	8.028	2803650	20.0