

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016832.D
 Acq On : 29 Aug 2023 15:04
 Operator : MA/JU
 Sample : PB155072BL
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK072

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016832.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	12	16	26	rVB	191451	250292	3.07%	0.238%
2	3.817	86	90	116	rBV	1963907	2923034	35.81%	2.781%
3	4.134	139	144	149	rBV	37119	55117	0.68%	0.052%
4	7.169	653	660	672	rBV	2152826	3364103	41.21%	3.200%
5	7.363	686	693	705	rBV	1773838	2713756	33.24%	2.581%
6	7.546	717	724	733	rBV	2096074	3276993	40.14%	3.117%
7	8.028	798	806	818	rBV	1780655	2807230	34.39%	2.670%
8	8.728	918	925	941	rBV	2507350	4069443	49.85%	3.871%
9	9.222	1001	1009	1023	rBV	1976322	3248254	39.79%	3.090%
10	9.940	1121	1131	1147	rBV	1643437	2652996	32.50%	2.524%
11	10.463	1211	1220	1234	rBV	2372576	3950761	48.40%	3.758%
12	10.857	1279	1287	1297	rBV	2483312	4131460	50.61%	3.930%
13	11.010	1305	1313	1332	rBV	2350524	4045509	49.56%	3.848%
14	12.434	1549	1555	1564	rBV2	42127	70830	0.87%	0.067%
15	12.646	1587	1591	1597	rBV8	5001	9134	0.11%	0.009%
16	13.528	1734	1741	1746	rBV	21305	35508	0.43%	0.034%
17	13.646	1754	1761	1766	rVB6	8028	13747	0.17%	0.013%
18	14.093	1830	1837	1849	rBV	4043232	5484112	67.18%	5.217%
19	14.381	1879	1886	1906	rBV	4767263	6866132	84.11%	6.531%
20	14.534	1910	1912	1920	rVB8	5604	10244	0.13%	0.010%
21	14.681	1930	1937	1952	rBV	3644490	5252080	64.34%	4.996%
22	14.887	1964	1972	1994	rBV	1276351	2333686	28.59%	2.220%
23	15.675	2099	2106	2120	rBV	5731929	8163490	100.00%	7.766%
24	15.798	2121	2127	2140	rVV	1364321	1938510	23.75%	1.844%
25	15.910	2143	2146	2155	rVB2	29286	46938	0.57%	0.045%
26	17.116	2346	2351	2356	rBV9	8941	16228	0.20%	0.015%
27	17.234	2367	2371	2375	rBV2	8673	11663	0.14%	0.011%
28	17.445	2401	2407	2417	rBV	3757228	5461499	66.90%	5.195%
29	17.545	2418	2424	2443	rVB	5361169	7873730	96.45%	7.490%
30	18.286	2547	2550	2556	rBV7	17255	31173	0.38%	0.030%
31	19.351	2728	2731	2737	rVB2	59534	81703	1.00%	0.078%
32	19.422	2740	2743	2748	rVB	58992	71637	0.88%	0.068%
33	19.780	2798	2804	2816	rBV	6073807	7766990	95.14%	7.388%
34	21.545	3099	3104	3113	rBV	3307121	4307312	52.76%	4.097%
35	23.945	3504	3512	3524	rVB2	3387570	7199072	88.19%	6.848%
36	24.116	3534	3541	3555	rVB	2100299	4590069	56.23%	4.366%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016832.D
Acq On : 29 Aug 2023 15:04
Operator : MA/JU
Sample : PB155072BL
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK072

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 105124435

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016832.D
Acq On : 29 Aug 2023 15:04
Operator : MA/JU
Sample : PB155072BL
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK072

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

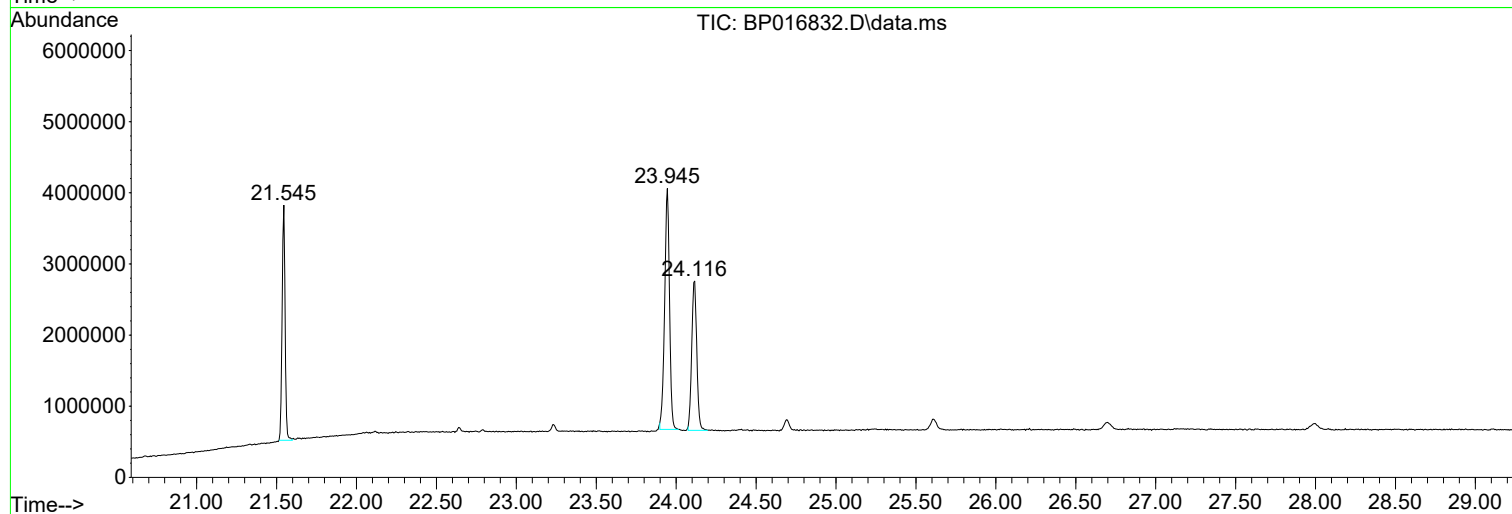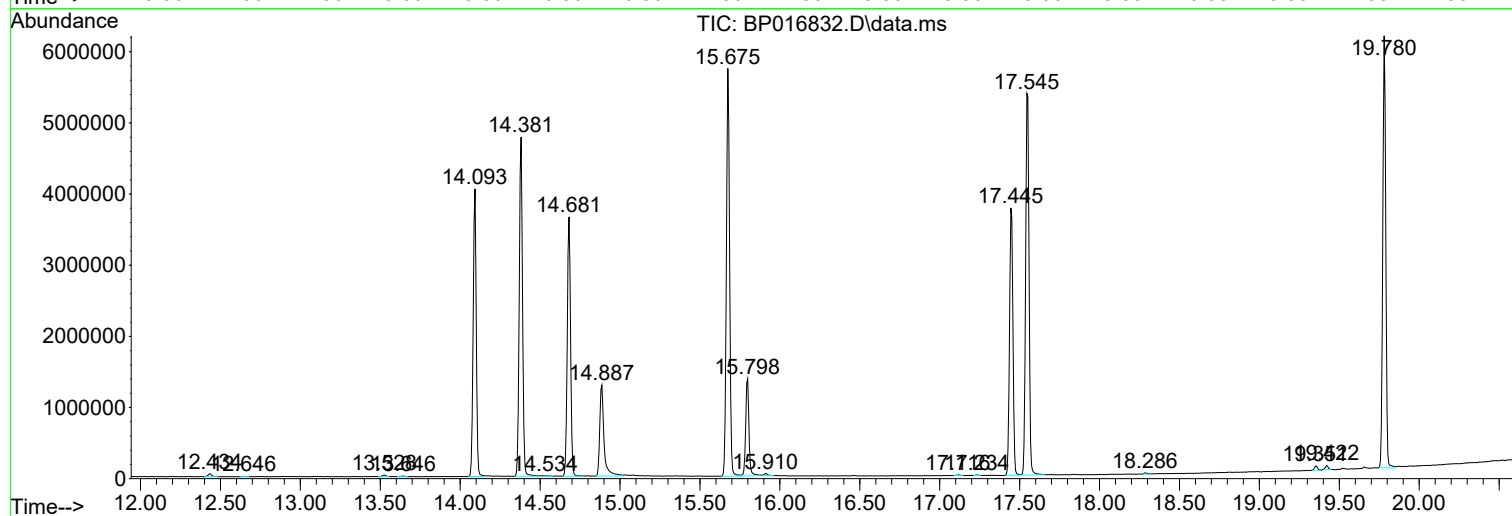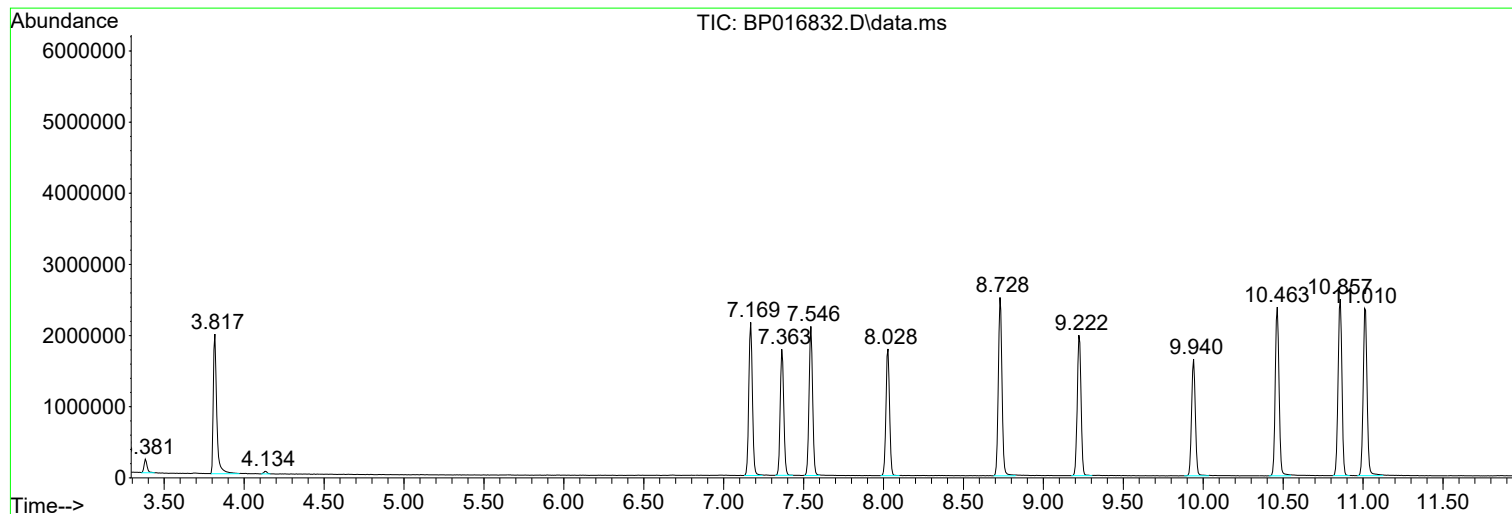

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016832.D
Acq On : 29 Aug 2023 15:04
Operator : MA/JU
Sample : PB155072BL
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK072

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016832.D
Acq On : 29 Aug 2023 15:04
Operator : MA/JU
Sample : PB155072BL
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK072

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------