

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016838.D
 Acq On : 29 Aug 2023 18:29
 Operator : MA/JU
 Sample : 04134-02DL 10X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCHJ0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016838.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	13	16	21	rBV3	12725	15711	0.30%	0.035%
2	3.828	89	92	101	rBV	44252	75258	1.43%	0.167%
3	4.128	139	143	150	rBV	57584	83647	1.59%	0.186%
4	5.987	455	459	465	rVB	15186	24191	0.46%	0.054%
5	7.169	653	660	671	rVB	46394	83277	1.58%	0.185%
6	7.363	685	693	703	rBV	208439	332537	6.33%	0.740%
7	7.546	711	724	735	rBV	175568	286388	5.45%	0.637%
8	7.640	735	740	747	rVV9	4831	10456	0.20%	0.023%
9	7.740	751	757	763	rVV	31361	49787	0.95%	0.111%
10	8.028	797	806	814	rBV	1410847	2202963	41.92%	4.899%
11	8.110	816	820	827	rVB3	10075	17740	0.34%	0.039%
12	8.563	891	897	903	rBV3	19847	36020	0.69%	0.080%
13	8.728	919	925	934	rBV	127835	215528	4.10%	0.479%
14	8.899	946	954	962	rBV	126216	202535	3.85%	0.450%
15	9.140	990	995	1001	rBV9	5694	11972	0.23%	0.027%
16	9.222	1001	1009	1017	rVV	202518	351505	6.69%	0.782%
17	9.387	1032	1037	1043	rVV5	10240	18140	0.35%	0.040%
18	9.463	1043	1050	1053	rVV5	14452	27176	0.52%	0.060%
19	9.516	1053	1059	1064	rVV3	19885	43181	0.82%	0.096%
20	9.575	1064	1069	1075	rVB2	13308	24194	0.46%	0.054%
21	9.940	1122	1131	1140	rBV	111892	195374	3.72%	0.434%
22	10.040	1144	1148	1154	rVV5	11276	22240	0.42%	0.049%
23	10.134	1157	1164	1171	rBV4	8990	17131	0.33%	0.038%
24	10.222	1171	1179	1181	rBV7	5568	9256	0.18%	0.021%
25	10.463	1212	1220	1227	rBV	232297	411324	7.83%	0.915%
26	10.604	1239	1244	1251	rVB9	6292	14799	0.28%	0.033%
27	10.769	1267	1272	1279	rVB8	6616	15306	0.29%	0.034%
28	10.857	1279	1287	1291	rBV	2008190	3378402	64.29%	7.513%
29	10.910	1291	1296	1303	rVV	3191039	5254562	100.00%	11.686%
30	11.028	1306	1316	1328	rVV2	427631	1018340	19.38%	2.265%
31	11.110	1328	1330	1337	rVV8	7178	13620	0.26%	0.030%
32	11.181	1337	1342	1347	rVV9	5466	12837	0.24%	0.029%
33	11.381	1371	1376	1381	rBV7	4722	8972	0.17%	0.020%
34	11.716	1428	1433	1435	rBV6	6189	8493	0.16%	0.019%
35	11.869	1453	1459	1463	rBV3	11632	19085	0.36%	0.042%
36	11.928	1463	1469	1472	rBV7	6617	12340	0.23%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016838.D
 Acq On : 29 Aug 2023 18:29
 Operator : MA/JU
 Sample : 04134-02DL 10X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCHJ0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

37	12.187	1508	1513	1520	rVB4	10075	18026	0.34%	0.040%
38	12.251	1520	1524	1526	rBV4	5141	8873	0.17%	0.020%
39	12.410	1545	1551	1560	rVB3	26383	61601	1.17%	0.137%
40	12.510	1561	1568	1577	rBV	301048	489659	9.32%	1.089%
41	12.634	1583	1589	1593	rBV5	12822	24355	0.46%	0.054%
42	12.728	1597	1605	1612	rVV	228546	383907	7.31%	0.854%
43	12.816	1615	1620	1625	rVV3	19785	31302	0.60%	0.070%
44	12.863	1625	1628	1641	rVB3	13625	31230	0.59%	0.069%
45	13.087	1660	1666	1669	rBV8	5943	10606	0.20%	0.024%
46	13.169	1674	1680	1683	rBV5	20095	41202	0.78%	0.092%
47	13.234	1688	1691	1699	rVB8	9476	17828	0.34%	0.040%
48	13.381	1708	1716	1719	rBV9	4788	12498	0.24%	0.028%
49	13.516	1733	1739	1752	rVB3	237788	391080	7.44%	0.870%
50	13.704	1766	1771	1779	rVB5	13567	33298	0.63%	0.074%
51	13.834	1787	1793	1795	rBV5	18456	32243	0.61%	0.072%
52	13.987	1814	1819	1825	rBV	33919	58078	1.11%	0.129%
53	14.045	1825	1829	1831	rVV2	15003	19721	0.38%	0.044%
54	14.087	1831	1836	1846	rVV	525777	743085	14.14%	1.653%
55	14.163	1846	1849	1856	rVB8	7422	12295	0.23%	0.027%
56	14.228	1856	1860	1864	rBV3	14149	19631	0.37%	0.044%
57	14.263	1864	1866	1874	rVB8	8852	11400	0.22%	0.025%
58	14.381	1878	1886	1897	rBV	580056	937115	17.83%	2.084%
59	14.681	1925	1937	1943	rBV	3087525	4469200	85.05%	9.939%
60	14.745	1943	1948	1956	rVV	422204	650419	12.38%	1.446%
61	14.828	1957	1962	1969	rVV	228959	354842	6.75%	0.789%
62	14.892	1971	1973	1980	rVB6	14633	21771	0.41%	0.048%
63	14.957	1980	1984	1995	rVB5	17557	40266	0.77%	0.090%
64	15.081	1999	2005	2019	rVB	503999	758362	14.43%	1.687%
65	15.210	2022	2027	2032	rBV2	84187	129644	2.47%	0.288%
66	15.292	2037	2041	2047	rVB3	34275	57889	1.10%	0.129%
67	15.675	2100	2106	2111	rBV	807024	1159563	22.07%	2.579%
68	15.728	2111	2115	2121	rVV	200104	311686	5.93%	0.693%
69	15.792	2121	2126	2133	rVV2	91923	145411	2.77%	0.323%
70	15.851	2133	2136	2143	rVB9	17386	30316	0.58%	0.067%
71	15.922	2143	2148	2151	rBV4	32284	53433	1.02%	0.119%
72	16.016	2161	2164	2174	rVB4	21354	50194	0.96%	0.112%
73	16.116	2176	2181	2184	rVV7	9499	18065	0.34%	0.040%
74	16.169	2186	2190	2200	rVB4	24701	54447	1.04%	0.121%
75	16.251	2201	2204	2208	rVB6	6409	9353	0.18%	0.021%
76	16.428	2227	2234	2245	rVB	69812	123586	2.35%	0.275%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016838.D
 Acq On : 29 Aug 2023 18:29
 Operator : MA/JU
 Sample : 04134-02DL 10X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCHJ0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

77	16.622	2262	2267	2272	rBV9	7477	12564	0.24%	0.028%
78	16.704	2275	2281	2286	rBV	136272	211797	4.03%	0.471%
79	16.945	2318	2322	2327	rBV8	8078	19202	0.37%	0.043%
80	17.069	2338	2343	2346	rBV3	141326	221018	4.21%	0.492%
81	17.104	2346	2349	2357	rVB	125334	182096	3.47%	0.405%
82	17.263	2373	2376	2381	rVB	32332	43689	0.83%	0.097%
83	17.339	2385	2389	2393	rVB2	11916	16092	0.31%	0.036%
84	17.398	2394	2399	2401	rBV	28065	36875	0.70%	0.082%
85	17.445	2401	2407	2412	rVV	3688575	5163897	98.27%	11.484%
86	17.492	2412	2415	2419	rVV	279469	420556	8.00%	0.935%
87	17.545	2419	2424	2439	rVB	864140	1289884	24.55%	2.869%
88	17.663	2441	2444	2448	rVV6	8020	11430	0.22%	0.025%
89	17.810	2465	2469	2472	rBV3	18674	25466	0.48%	0.057%
90	17.863	2472	2478	2491	rVV	1261949	1718316	32.70%	3.821%
91	18.010	2498	2503	2512	rBV	130738	222547	4.24%	0.495%
92	18.281	2546	2549	2556	rVB7	24148	41176	0.78%	0.092%
93	18.351	2558	2561	2567	rVV4	24495	36246	0.69%	0.081%
94	18.645	2609	2611	2614	rBV	11633	11830	0.23%	0.026%
95	18.739	2624	2627	2632	rVB4	24101	27948	0.53%	0.062%
96	18.786	2632	2635	2640	rBV4	15536	24659	0.47%	0.055%
97	19.657	2780	2783	2787	rVB2	52422	49371	0.94%	0.110%
98	19.780	2799	2804	2810	rBV	934045	1245022	23.69%	2.769%
99	21.545	3099	3104	3111	rBV	2866220	3844635	73.17%	8.550%
100	24.110	3534	3540	3551	rVB	1760719	3737214	71.12%	8.311%




Sum of corrected areas: 44965297

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016838.D
Acq On : 29 Aug 2023 18:29
Operator : MA/JU
Sample : 04134-02DL 10X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHJ0DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

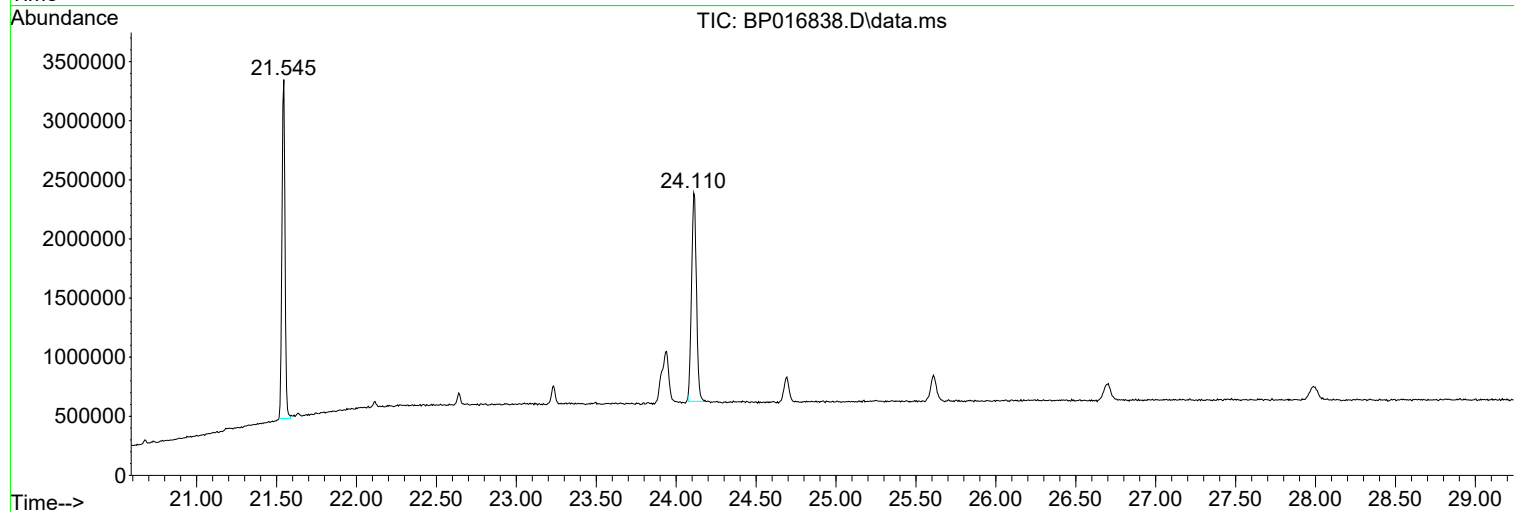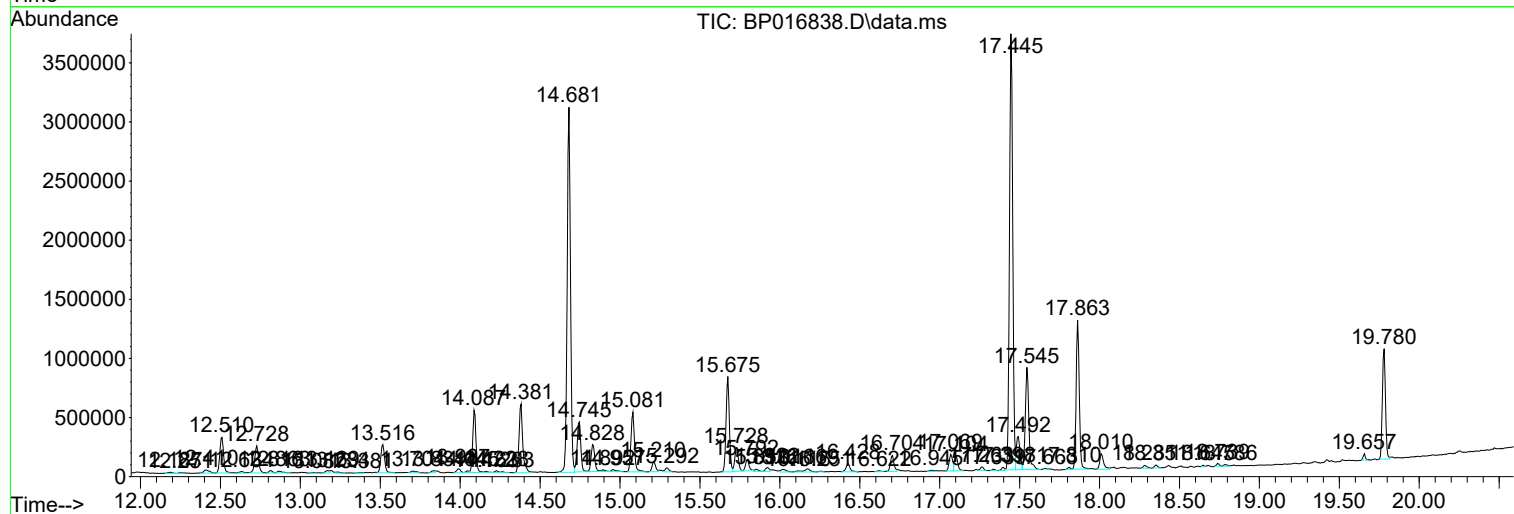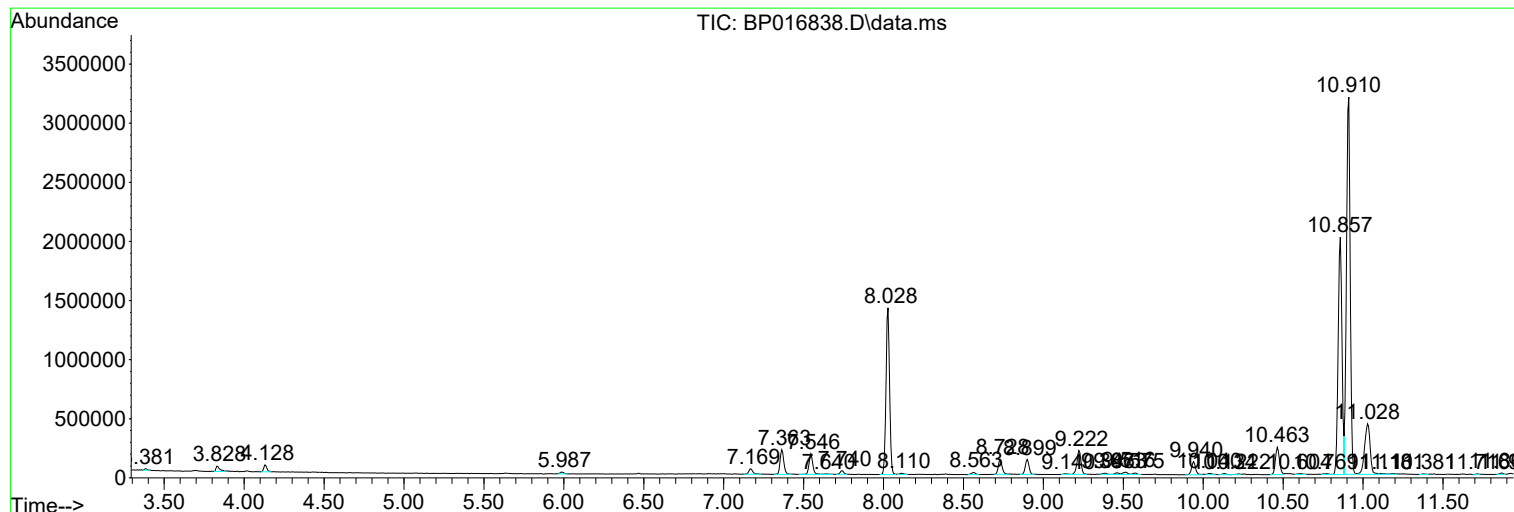

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016838.D
Acq On : 29 Aug 2023 18:29
Operator : MA/JU
Sample : 04134-02DL 10X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHJ0DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016838.D
Acq On : 29 Aug 2023 18:29
Operator : MA/JU
Sample : 04134-02DL 10X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHJ0DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc