

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016850.D
 Acq On : 30 Aug 2023 01:52
 Operator : MA/JU
 Sample : PB155157BL
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK157

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016850.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	12	16	28	rVB	170564	250975	1.73%	0.169%
2	3.817	85	90	115	rBV	1569021	2560438	17.63%	1.728%
3	4.128	139	143	152	rVB	42844	63775	0.44%	0.043%
4	7.169	653	660	673	rBV	2737143	4347925	29.94%	2.934%
5	7.364	686	693	702	rVB	2261632	3442296	23.70%	2.323%
6	7.546	716	724	736	rBV	2643353	4224236	29.08%	2.851%
7	8.022	797	805	818	rVB	1964005	3158778	21.75%	2.132%
8	8.728	917	925	938	rBV	3391134	5400852	37.19%	3.645%
9	9.222	1001	1009	1021	rBV	2649765	4256755	29.31%	2.873%
10	9.940	1121	1131	1140	rBV	2103637	3465683	23.86%	2.339%
11	10.457	1212	1219	1240	rBV	3206229	5453818	37.55%	3.680%
12	10.852	1277	1286	1296	rBV	2878746	4862664	33.48%	3.281%
13	11.010	1305	1313	1326	rBV	1561049	2656369	18.29%	1.793%
14	12.434	1550	1555	1562	rVB2	56564	95493	0.66%	0.064%
15	13.522	1735	1740	1748	rBV	47249	70969	0.49%	0.048%
16	14.093	1830	1837	1848	rBV	6011080	8280294	57.01%	5.588%
17	14.381	1878	1886	1900	rBV	6631887	10078436	69.39%	6.801%
18	14.675	1930	1936	1947	rBV	4554140	6759315	46.54%	4.561%
19	14.881	1964	1971	1995	rBV	2326165	3948681	27.19%	2.665%
20	15.075	2002	2004	2012	rVB9	13322	15198	0.10%	0.010%
21	15.675	2098	2106	2120	rBV	8677565	12503128	86.09%	8.437%
22	15.792	2120	2126	2139	rVV	2369067	3157147	21.74%	2.130%
23	15.910	2142	2146	2157	rVB	43237	77845	0.54%	0.053%
24	16.457	2236	2239	2245	rVB6	8728	14574	0.10%	0.010%
25	17.228	2367	2370	2374	rVB3	10604	15494	0.11%	0.010%
26	17.445	2400	2407	2417	rBV	5790845	7988323	55.00%	5.391%
27	17.545	2417	2424	2442	rVV	9969814	13633160	93.87%	9.200%
28	18.075	2510	2514	2519	rBV8	17410	23245	0.16%	0.016%
29	18.281	2545	2549	2557	rBV6	35439	60673	0.42%	0.041%
30	19.351	2727	2731	2735	rBV2	113722	142091	0.98%	0.096%
31	19.416	2738	2742	2748	rVB	97978	135751	0.93%	0.092%
32	19.516	2756	2759	2764	rBV4	34577	44458	0.31%	0.030%
33	19.781	2798	2804	2810	rBV	11591974	14523995	100.00%	9.801%
34	21.539	3098	3103	3113	rBV	4956135	6445784	44.38%	4.350%
35	23.939	3503	3511	3528	rVB2	5008437	10406363	71.65%	7.022%
36	24.110	3532	3540	3554	rVB	2624084	5623857	38.72%	3.795%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016850.D
Acq On : 30 Aug 2023 01:52
Operator : MA/JU
Sample : PB155157BL
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK157

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 148188838

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016850.D
Acq On : 30 Aug 2023 01:52
Operator : MA/JU
Sample : PB155157BL
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK157

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

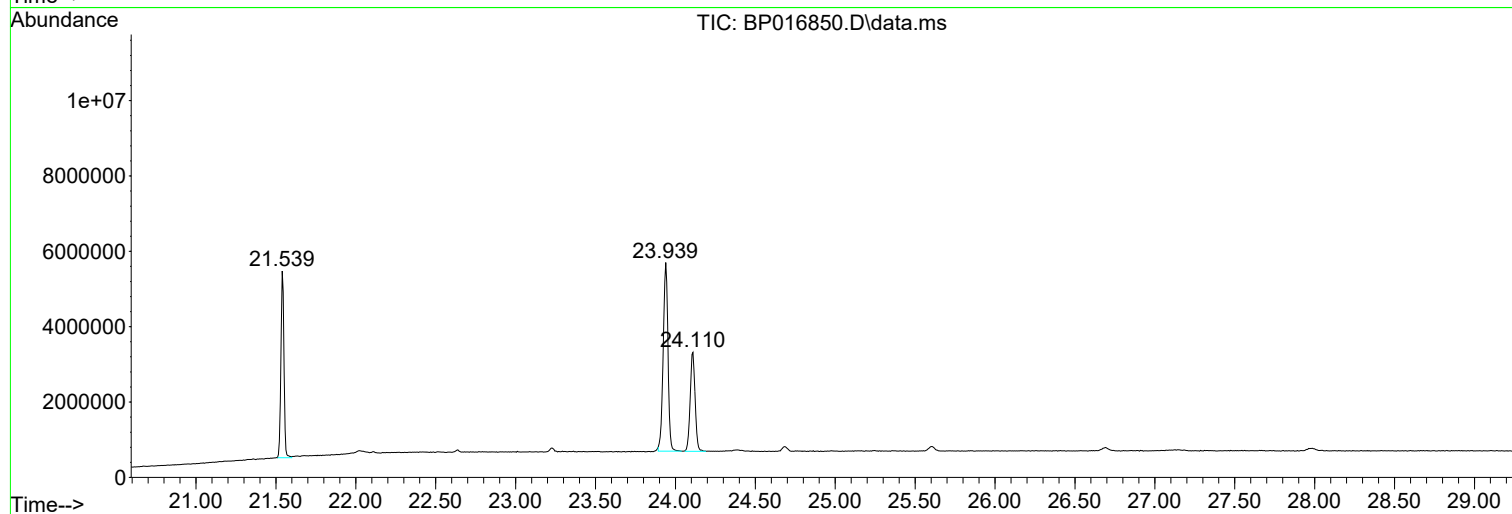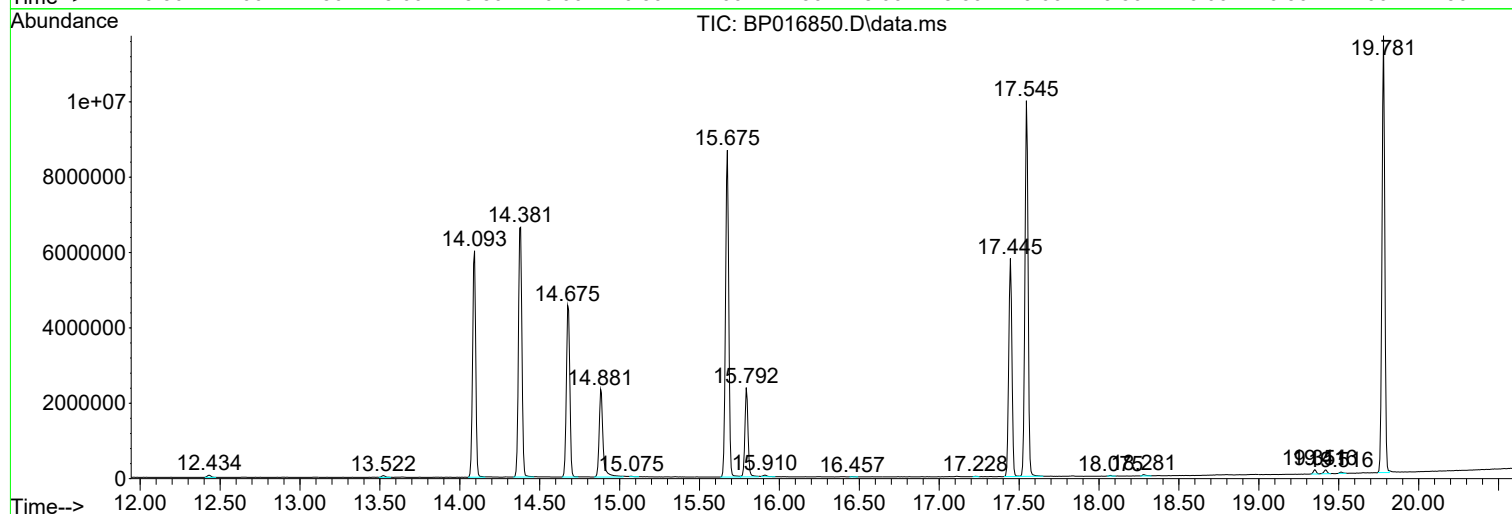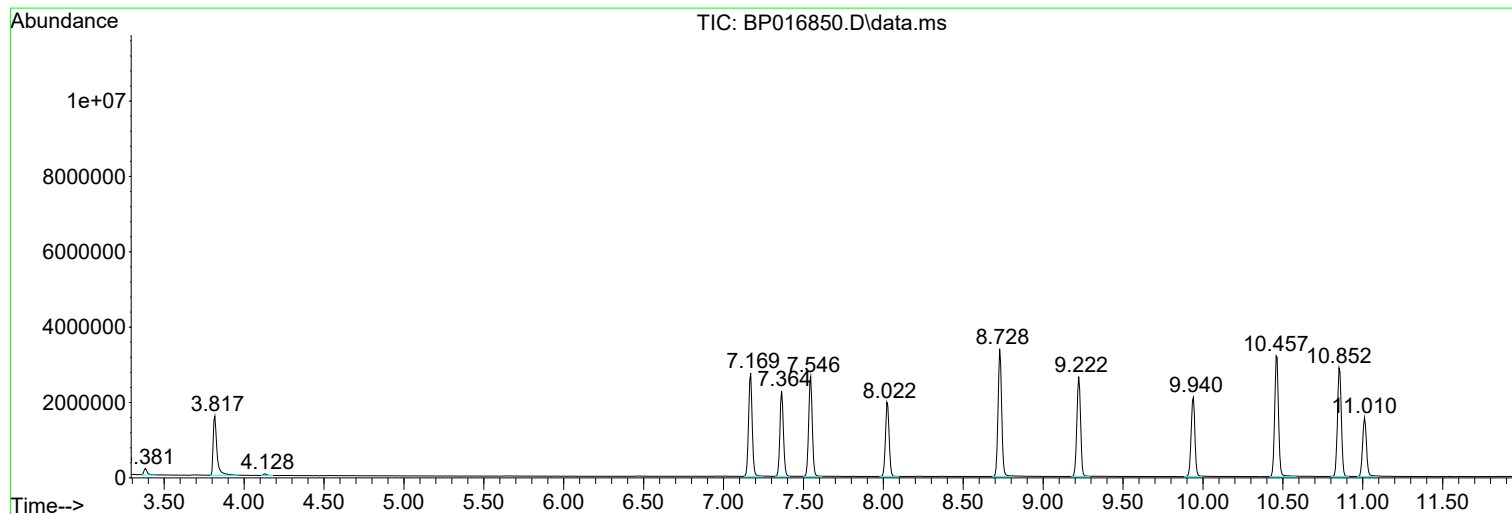

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016850.D
Acq On : 30 Aug 2023 01:52
Operator : MA/JU
Sample : PB155157BL
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK157

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016850.D
Acq On : 30 Aug 2023 01:52
Operator : MA/JU
Sample : PB155157BL
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK157

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------