

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016853.D
 Acq On : 30 Aug 2023 03:34
 Operator : MA/JU
 Sample : 04148-10
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBKG5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016853.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	3	8	20	rBV	1693820	2885759	3.55%	1.310%
2	3.417	20	22	31	rVB	79398	117412	0.14%	0.053%
3	3.817	87	90	104	rBV	483625	794971	0.98%	0.361%
4	4.017	119	124	130	rVB	53430	85809	0.11%	0.039%
5	4.134	139	144	152	rVB	61656	97361	0.12%	0.044%
6	4.658	226	233	238	rBV2	33157874	81400053	100.00%	36.959%
7	6.711	577	582	591	rBV	53543	83977	0.10%	0.038%
8	7.169	654	660	672	rVB	528696	873527	1.07%	0.397%
9	7.364	686	693	706	rVB	2143073	3294020	4.05%	1.496%
10	7.546	715	724	736	rBV	1922983	3143888	3.86%	1.427%
11	8.022	798	805	820	rBV	1622027	2620157	3.22%	1.190%
12	8.728	918	925	934	rBV	1715847	2687639	3.30%	1.220%
13	8.810	934	939	952	rVV	36183	95470	0.12%	0.043%
14	9.222	1000	1009	1019	rBV	2563345	4194041	5.15%	1.904%
15	9.934	1123	1130	1139	rBV	1968635	3201510	3.93%	1.454%
16	10.457	1211	1219	1240	rBV	2972397	5092084	6.26%	2.312%
17	10.852	1279	1286	1294	rBV	2382147	3961952	4.87%	1.799%
18	11.010	1305	1313	1323	rBV	873094	1487786	1.83%	0.676%
19	12.428	1547	1554	1562	rBV2	58574	120457	0.15%	0.055%
20	13.522	1732	1740	1745	rBV3	70375	140715	0.17%	0.064%
21	13.657	1757	1763	1773	rBV3	85262	162089	0.20%	0.074%
22	14.093	1830	1837	1843	rBV	6298234	8666292	10.65%	3.935%
23	14.381	1878	1886	1903	rBV	6714635	10297271	12.65%	4.675%
24	14.581	1913	1920	1928	rBV	215363	358333	0.44%	0.163%
25	14.675	1930	1936	1944	rVV	3510613	5247229	6.45%	2.382%
26	14.887	1964	1972	1983	rBV2	395162	749657	0.92%	0.340%
27	15.216	2024	2028	2034	rBV2	64708	110692	0.14%	0.050%
28	15.675	2099	2106	2112	rBV	9215859	13050451	16.03%	5.925%
29	15.734	2112	2116	2121	rVV	242657	369376	0.45%	0.168%
30	15.792	2121	2126	2139	rVB	2770516	3906582	4.80%	1.774%
31	15.910	2141	2146	2148	rBV3	56001	92195	0.11%	0.042%
32	16.398	2224	2229	2235	rBV	296989	410935	0.50%	0.187%
33	17.445	2401	2407	2417	rBV	4510798	6233516	7.66%	2.830%
34	17.545	2418	2424	2440	rVV2	10123099	14845054	18.24%	6.740%
35	18.281	2545	2549	2560	rBV	368169	611129	0.75%	0.277%
36	19.351	2727	2731	2735	rBV	146039	186853	0.23%	0.085%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016853.D
Acq On : 30 Aug 2023 03:34
Operator : MA/JU
Sample : 04148-10
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBKG5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Title : SVOA CALIBRATION

37	19.416	2739	2742	2747	rVB	128727	177011	0.22%	0.080%
38	19.516	2755	2759	2771	rBV2	292745	480154	0.59%	0.218%
39	19.781	2798	2804	2815	rBV	12133105	16327464	20.06%	7.413%
40	21.539	3098	3103	3113	rBV2	4008498	5318894	6.53%	2.415%
41	23.939	3502	3511	3523	rVB2	5419379	11845848	14.55%	5.378%
42	24.110	3533	3540	3549	rVB	2065808	4420654	5.43%	2.007%




Sum of corrected areas: 220246267

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016853.D
Acq On : 30 Aug 2023 03:34
Operator : MA/JU
Sample : 04148-10
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBKG5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

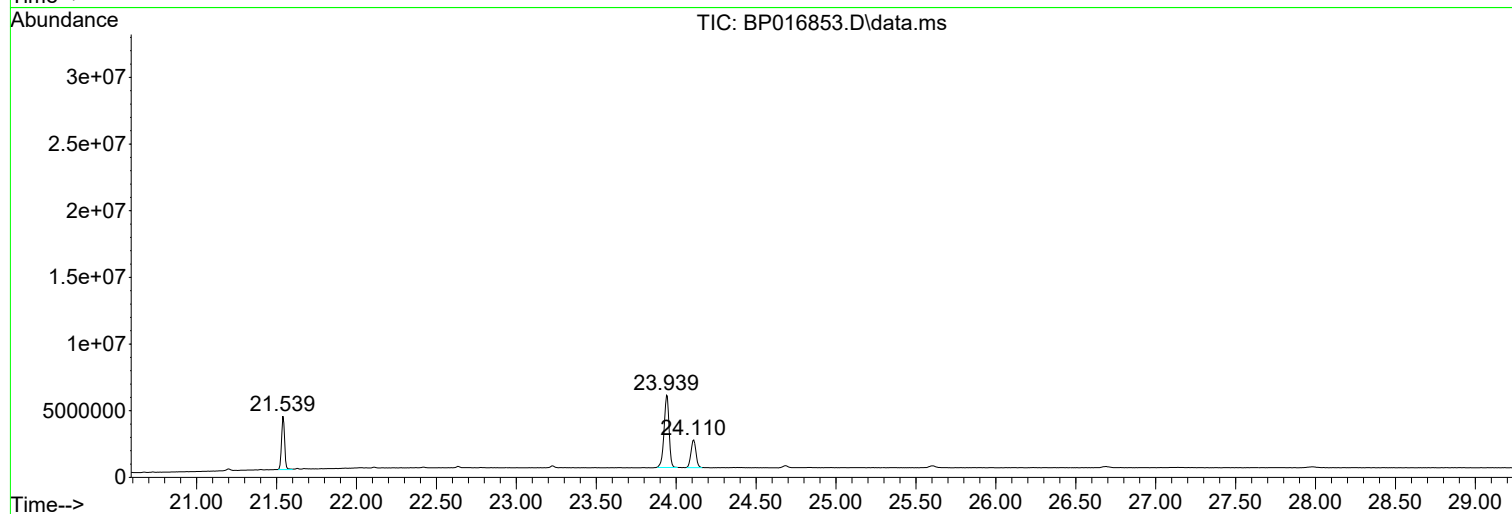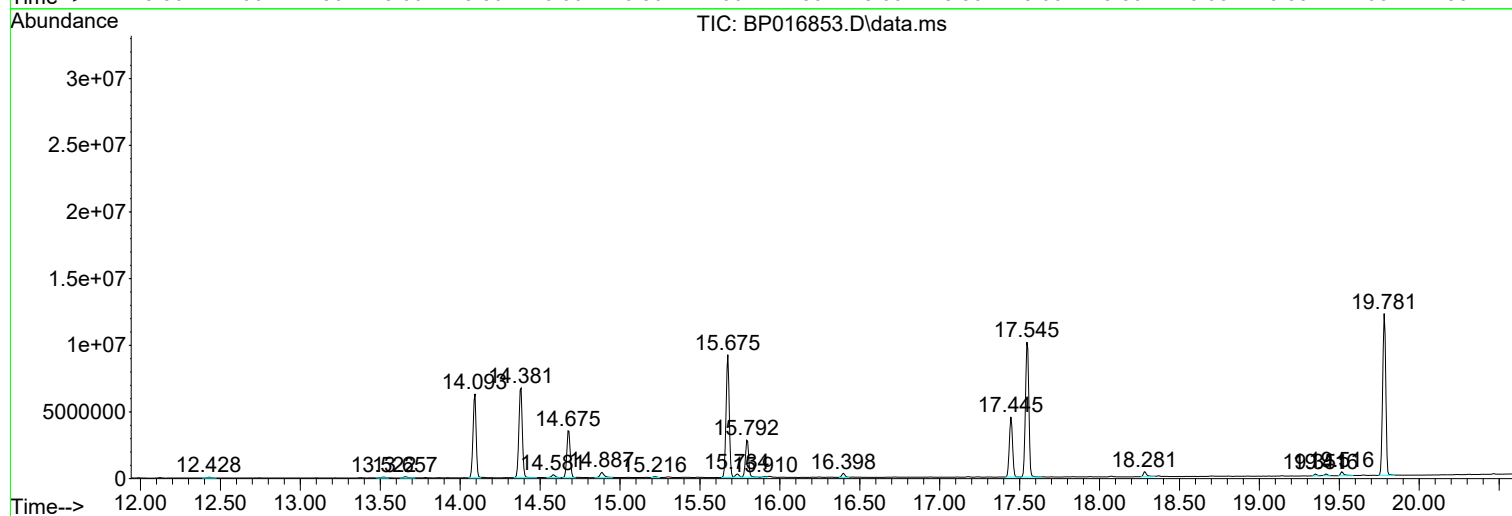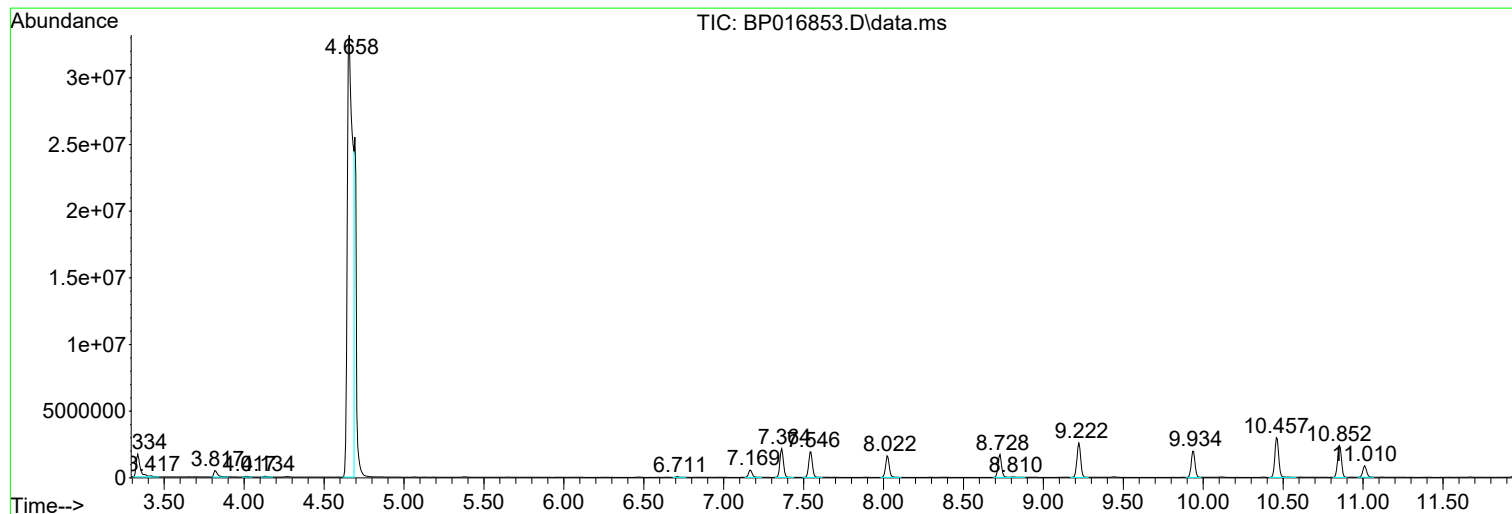

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016853.D
Acq On : 30 Aug 2023 03:34
Operator : MA/JU
Sample : 04148-10
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBKG5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.658	621.34 ng/ul	81400100	1,4-Dichlorobenzene-d4	8.022

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
5			2,4-Dichloro-6-fluoropyrimidine	166	C4HC12FN2	003833-57-6	38

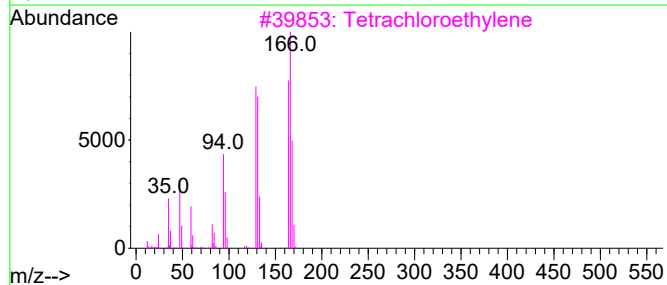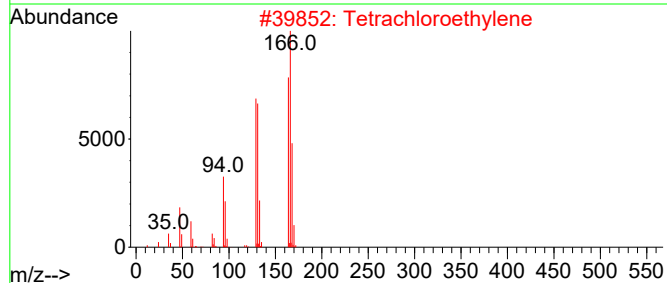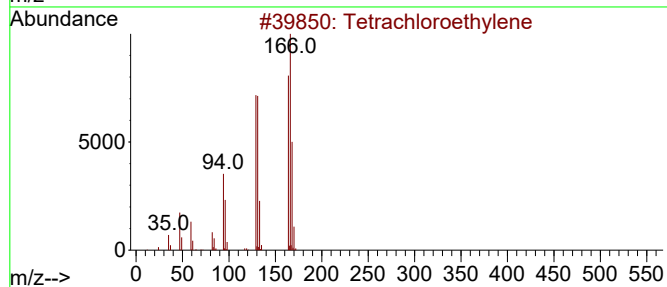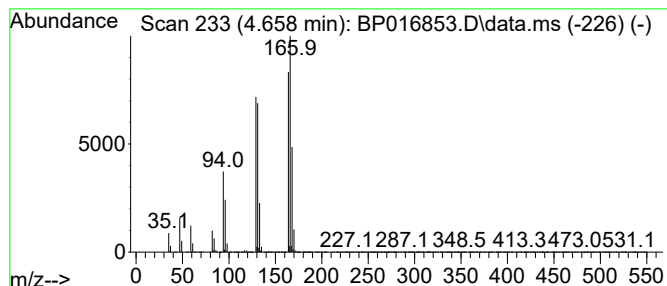

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016853.D
Acq On : 30 Aug 2023 03:34
Operator : MA/JU
Sample : 04148-10
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBKG5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.658	621.3	ng/ul	81400100	1	8.022	2620160	20.0