

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016856.D
 Acq On : 30 Aug 2023 05:16
 Operator : MA/JU
 Sample : 04159-09
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCHK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016856.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	12	16	23	rVB	107574	137612	0.97%	0.110%
2	3.693	65	69	79	rVB5	14360	33245	0.23%	0.027%
3	3.817	87	90	106	rBV	590620	941827	6.65%	0.753%
4	4.017	118	124	131	rVB	50988	87638	0.62%	0.070%
5	4.128	139	143	155	rVB	112082	171624	1.21%	0.137%
6	5.069	297	303	307	rBV2	18129	27341	0.19%	0.022%
7	5.652	397	402	407	rVB3	9032	14237	0.10%	0.011%
8	6.963	620	625	630	rBV7	7230	14579	0.10%	0.012%
9	7.163	652	659	668	rBV	403863	657215	4.64%	0.526%
10	7.363	685	693	702	rBV	1833480	2809706	19.83%	2.248%
11	7.540	716	723	734	rBV	1579865	2542440	17.95%	2.034%
12	8.022	798	805	817	rBV	1731874	2771576	19.56%	2.217%
13	8.563	890	897	902	rBV5	11400	19565	0.14%	0.016%
14	8.728	918	925	937	rBV	1254192	2012739	14.21%	1.610%
15	8.899	950	954	960	rVB	18244	29472	0.21%	0.024%
16	9.140	988	995	1001	rBV5	9461	18462	0.13%	0.015%
17	9.222	1001	1009	1024	rVV	2177268	3542710	25.01%	2.834%
18	9.446	1041	1047	1051	rBV4	9585	16135	0.11%	0.013%
19	9.934	1120	1130	1145	rBV	1676167	2731295	19.28%	2.185%
20	10.252	1179	1184	1192	rVB5	11752	23659	0.17%	0.019%
21	10.457	1211	1219	1228	rBV	2318860	3933668	27.77%	3.147%
22	10.704	1256	1261	1267	rVB2	16119	29686	0.21%	0.024%
23	10.852	1278	1286	1294	rBV	2546432	4251028	30.01%	3.401%
24	11.010	1305	1313	1326	rBV2	2054381	3705698	26.16%	2.965%
25	11.240	1348	1352	1359	rVB5	17120	31337	0.22%	0.025%
26	11.451	1383	1388	1396	rVB2	21785	40940	0.29%	0.033%
27	11.669	1420	1425	1431	rVB6	12715	18102	0.13%	0.014%
28	11.934	1464	1470	1474	rBV3	19036	32237	0.23%	0.026%
29	12.010	1479	1483	1489	rVB4	7435	15123	0.11%	0.012%
30	12.428	1546	1554	1562	rBV3	47158	88281	0.62%	0.071%
31	12.640	1585	1590	1596	rBV10	6231	15598	0.11%	0.012%
32	12.740	1604	1607	1614	rVB7	12922	25072	0.18%	0.020%
33	12.810	1614	1619	1623	rBV2	22198	36447	0.26%	0.029%
34	12.857	1623	1627	1637	rVB9	22315	51761	0.37%	0.041%
35	13.028	1647	1656	1661	rBV9	11906	27683	0.20%	0.022%
36	13.375	1708	1715	1718	rBV9	8517	18433	0.13%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016856.D
 Acq On : 30 Aug 2023 05:16
 Operator : MA/JU
 Sample : 04159-09
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCHK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

37	13.522	1734	1740	1748	rBV	47429	79716	0.56%	0.064%
38	13.693	1764	1769	1775	rVB4	13940	25415	0.18%	0.020%
39	13.828	1787	1792	1797	rBV7	9820	17055	0.12%	0.014%
40	14.093	1829	1837	1850	rBV	4959846	7022820	49.57%	5.618%
41	14.375	1878	1885	1903	rBV	5523081	8235154	58.13%	6.588%
42	14.634	1924	1929	1930	rBV3	14240	19653	0.14%	0.016%
43	14.675	1930	1936	1950	rVB	3788907	5746965	40.57%	4.598%
44	14.828	1960	1962	1966	rVB2	17600	18205	0.13%	0.015%
45	14.887	1966	1972	1983	rBV	249053	495990	3.50%	0.397%
46	15.051	1995	2000	2003	rBV6	17522	25568	0.18%	0.020%
47	15.210	2022	2027	2031	rBV	73340	101488	0.72%	0.081%
48	15.298	2036	2042	2043	rBV5	21551	36160	0.26%	0.029%
49	15.410	2056	2061	2066	rVB4	18527	34348	0.24%	0.027%
50	15.675	2096	2106	2112	rBV	7749691	11045422	77.97%	8.836%
51	15.734	2112	2116	2120	rVV	256120	411057	2.90%	0.329%
52	15.792	2120	2126	2141	rVV	2313247	3251404	22.95%	2.601%
53	15.916	2142	2147	2156	rVB2	94179	167562	1.18%	0.134%
54	16.175	2188	2191	2200	rVB6	18786	39395	0.28%	0.032%
55	16.251	2200	2204	2209	rBV7	8670	16119	0.11%	0.013%
56	16.451	2234	2238	2244	rVB4	25663	41548	0.29%	0.033%
57	17.069	2338	2343	2347	rBV2	64519	97034	0.68%	0.078%
58	17.234	2367	2371	2373	rBV3	13245	17845	0.13%	0.014%
59	17.445	2401	2407	2417	rBV	4952357	6798833	47.99%	5.439%
60	17.545	2417	2424	2439	rBV2	9120977	12879183	90.91%	10.303%
61	17.804	2464	2468	2471	rBV	34728	50205	0.35%	0.040%
62	18.075	2510	2514	2522	rBV9	31386	55770	0.39%	0.045%
63	18.157	2524	2528	2532	rVV5	18320	28730	0.20%	0.023%
64	18.281	2545	2549	2560	rBV	316287	478686	3.38%	0.383%
65	19.351	2727	2731	2735	rBV3	103074	130406	0.92%	0.104%
66	19.416	2738	2742	2747	rVB	105006	140961	0.99%	0.113%
67	19.516	2755	2759	2763	rBV2	266370	361848	2.55%	0.289%
68	19.651	2780	2782	2786	rVB	34605	33581	0.24%	0.027%
69	19.780	2798	2804	2815	rBV	11245137	14166945	100.00%	11.334%
70	21.398	3077	3079	3085	rVB	132793	131704	0.93%	0.105%
71	21.539	3098	3103	3114	rBV2	4272097	5766393	40.70%	4.613%
72	22.421	3249	3253	3258	rVB	376819	483314	3.41%	0.387%
73	23.939	3503	3511	3526	rVB2	4857706	10551027	74.48%	8.441%
74	24.110	3533	3540	3553	rVB	2394988	5071326	35.80%	4.057%

Sum of corrected areas: 124999006




Instrument :
BNA_P
ClientSampleId :
DCHK3

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016856.D
Acq On : 30 Aug 2023 05:16
Operator : MA/JU
Sample : 04159-09
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHK3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

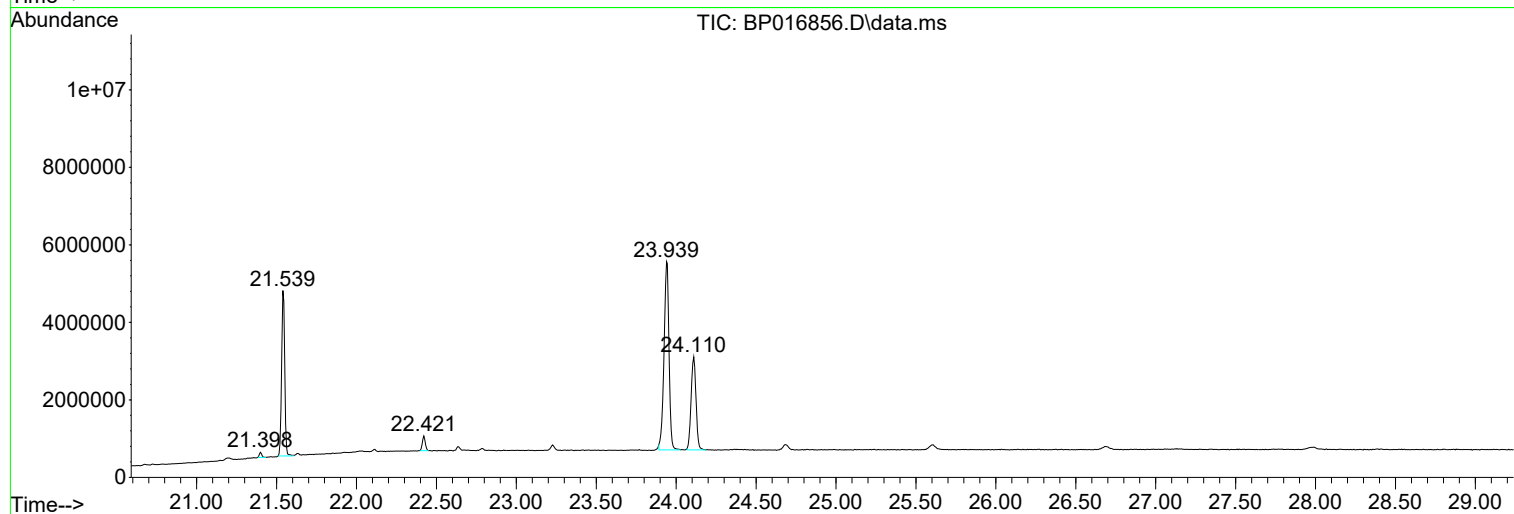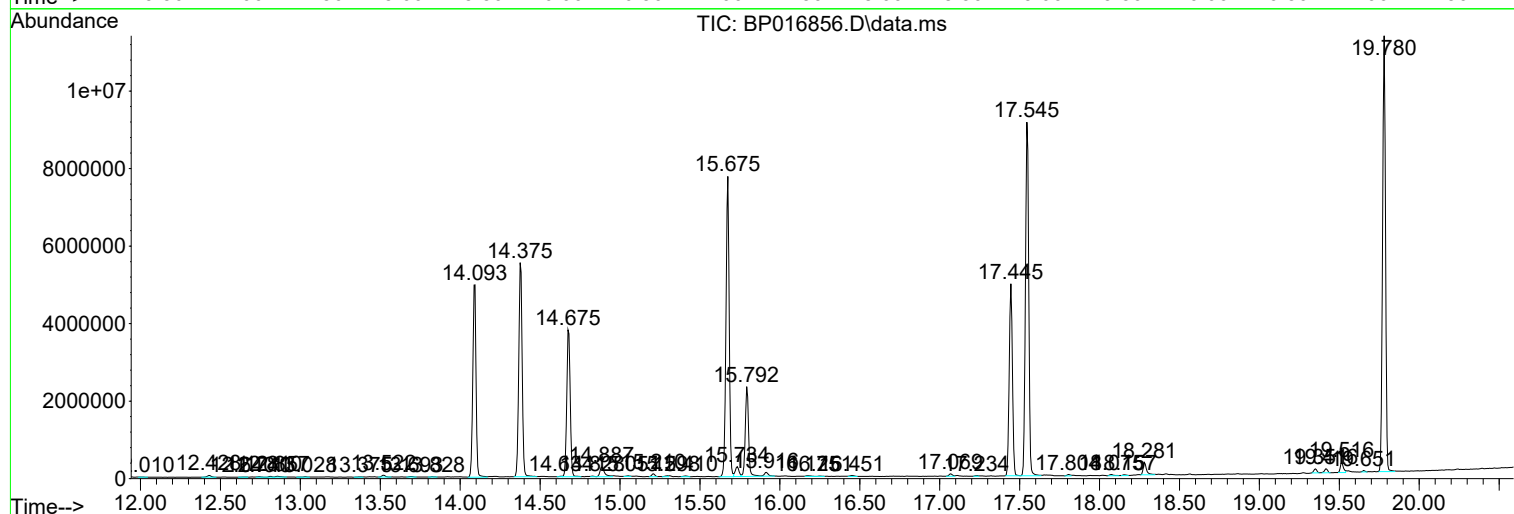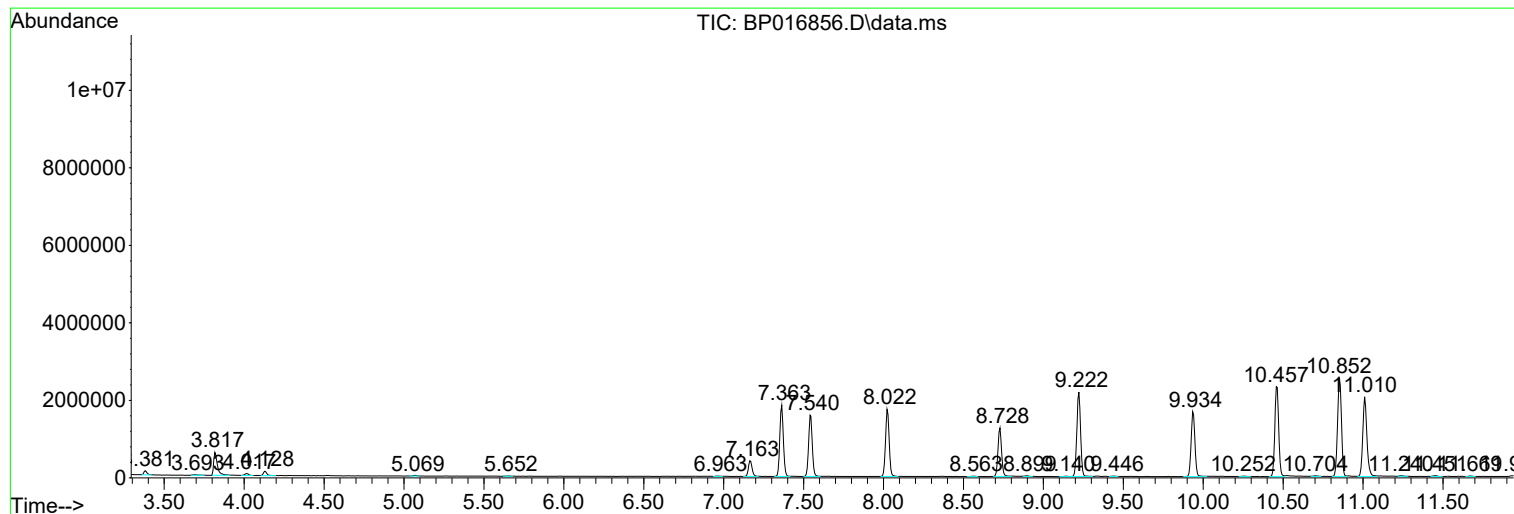

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016856.D
Acq On : 30 Aug 2023 05:16
Operator : MA/JU
Sample : 04159-09
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHK3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016856.D
Acq On : 30 Aug 2023 05:16
Operator : MA/JU
Sample : 04159-09
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHK3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc