

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016858.D
 Acq On : 30 Aug 2023 06:24
 Operator : MA/JU
 Sample : 04159-11
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCHL0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016858.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	12	16	26	rVB	80905	127102	1.03%	0.120%
2	3.687	66	68	75	rVB4	16537	26658	0.22%	0.025%
3	3.817	87	90	105	rBV	271406	478171	3.89%	0.451%
4	4.017	119	124	131	rVB	45995	74502	0.61%	0.070%
5	4.128	139	143	150	rVB	98388	143797	1.17%	0.136%
6	4.523	207	210	218	rVB10	8143	16783	0.14%	0.016%
7	5.070	295	303	309	rBV	14142	25620	0.21%	0.024%
8	5.264	331	336	341	rVB5	10089	17435	0.14%	0.016%
9	5.652	399	402	409	rVB5	9614	16350	0.13%	0.015%
10	7.164	653	659	671	rBV	347479	554511	4.51%	0.523%
11	7.364	684	693	702	rBV	1602375	2520603	20.51%	2.377%
12	7.540	716	723	734	rBV	1386618	2226000	18.11%	2.099%
13	8.022	798	805	820	rVB	1576004	2458662	20.00%	2.319%
14	8.728	918	925	936	rBV	1030935	1698363	13.82%	1.602%
15	9.222	1001	1009	1022	rBV	1916264	3145571	25.59%	2.967%
16	9.440	1042	1046	1050	rVB	10180	16203	0.13%	0.015%
17	9.934	1121	1130	1141	rBV	1460200	2374726	19.32%	2.240%
18	10.458	1212	1219	1233	rBV	2051677	3440152	27.99%	3.244%
19	10.852	1278	1286	1301	rVB	2294523	3805543	30.96%	3.589%
20	11.010	1305	1313	1333	rBV	1771053	3065015	24.94%	2.891%
21	11.669	1420	1425	1430	rBV5	12538	21777	0.18%	0.021%
22	11.934	1464	1470	1476	rVB2	23737	37235	0.30%	0.035%
23	12.428	1548	1554	1560	rBV	39968	69188	0.56%	0.065%
24	12.640	1584	1590	1597	rBV5	8521	20680	0.17%	0.020%
25	13.522	1733	1740	1746	rBV	48705	81194	0.66%	0.077%
26	13.640	1752	1760	1765	rVB9	8361	19557	0.16%	0.018%
27	14.087	1830	1836	1851	rBV	4540622	6226894	50.66%	5.873%
28	14.375	1878	1885	1906	rBV	4937174	7362616	59.90%	6.944%
29	14.675	1929	1936	1944	rBV	3521716	5141163	41.83%	4.849%
30	14.887	1966	1972	1986	rBV	178779	400251	3.26%	0.377%
31	15.310	2040	2044	2049	rBV5	16535	27002	0.22%	0.025%
32	15.416	2058	2062	2066	rVB3	9108	15253	0.12%	0.014%
33	15.487	2069	2074	2079	rVB8	10088	14597	0.12%	0.014%
34	15.675	2098	2106	2113	rBV	6695099	9620288	78.27%	9.073%
35	15.734	2113	2116	2120	rVV5	53047	92399	0.75%	0.087%
36	15.793	2120	2126	2141	rVV	1800779	2513401	20.45%	2.370%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016858.D
 Acq On : 30 Aug 2023 06:24
 Operator : MA/JU
 Sample : 04159-11
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCHL0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

37	15.910	2142	2146	2152	rVB2	31777	53304	0.43%	0.050%
38	16.257	2200	2205	2211	rVB10	7603	14348	0.12%	0.014%
39	17.110	2347	2350	2354	rBV5	8472	12340	0.10%	0.012%
40	17.228	2365	2370	2376	rBV4	10720	19329	0.16%	0.018%
41	17.445	2400	2407	2417	rBV	4439158	6121459	49.81%	5.773%
42	17.545	2417	2424	2436	rBV	8086233	11319000	92.10%	10.675%
43	18.075	2510	2514	2517	rBV5	27671	33564	0.27%	0.032%
44	18.281	2546	2549	2554	rBV2	35250	49505	0.40%	0.047%
45	19.351	2727	2731	2736	rVB	92919	111204	0.90%	0.105%
46	19.422	2739	2743	2747	rVB	79107	106370	0.87%	0.100%
47	19.516	2756	2759	2764	rBV5	27817	38774	0.32%	0.037%
48	19.781	2798	2804	2817	rBV	9821483	12290549	100.00%	11.591%
49	21.539	3098	3103	3111	rBV	3696393	5013315	40.79%	4.728%
50	23.939	3503	3511	3523	rVB2	4188321	8644617	70.34%	8.153%
51	24.110	3533	3540	3552	rVB	2010940	4308255	35.05%	4.063%




Sum of corrected areas: 106031195

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016858.D
Acq On : 30 Aug 2023 06:24
Operator : MA/JU
Sample : 04159-11
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHL0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

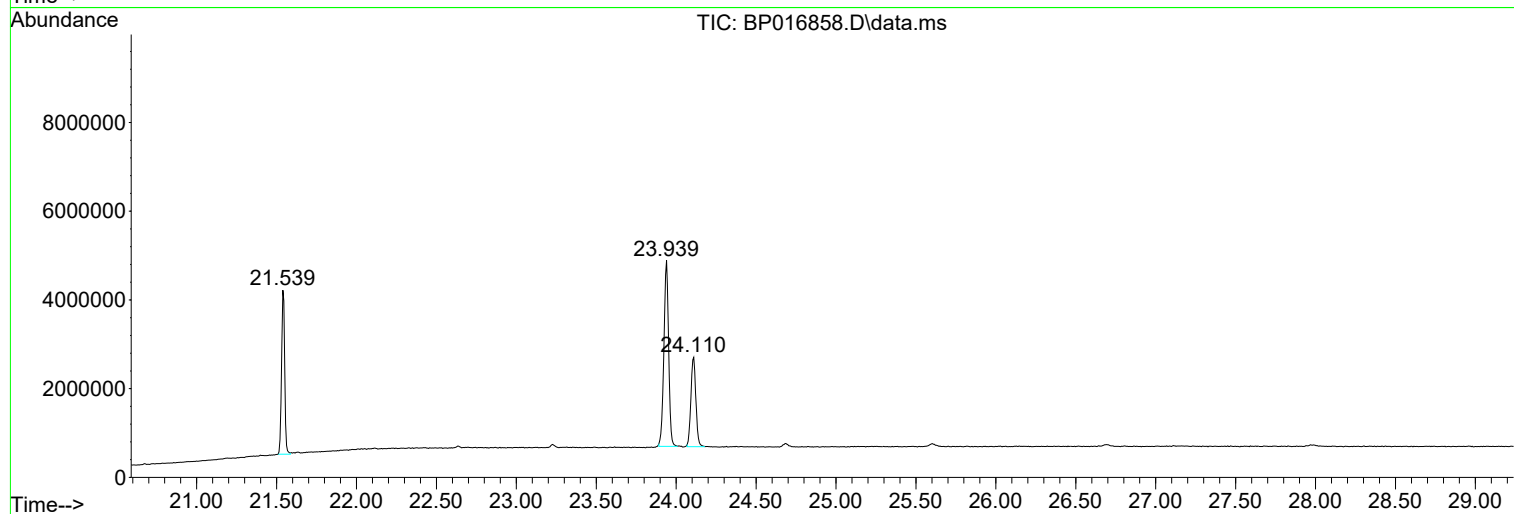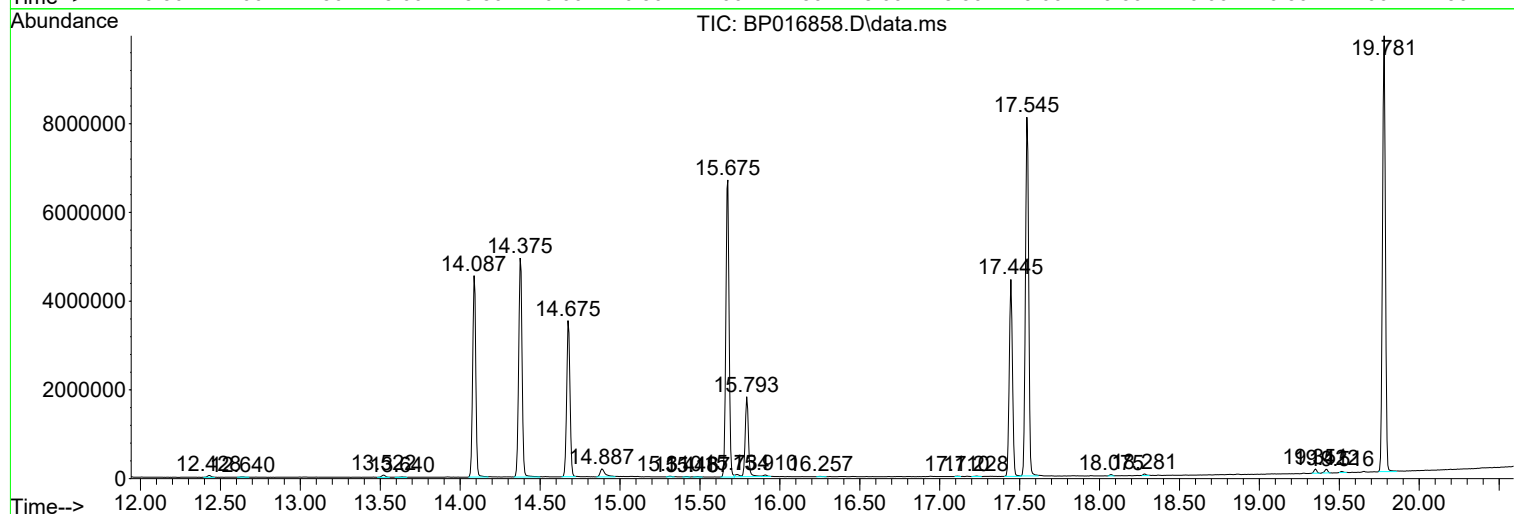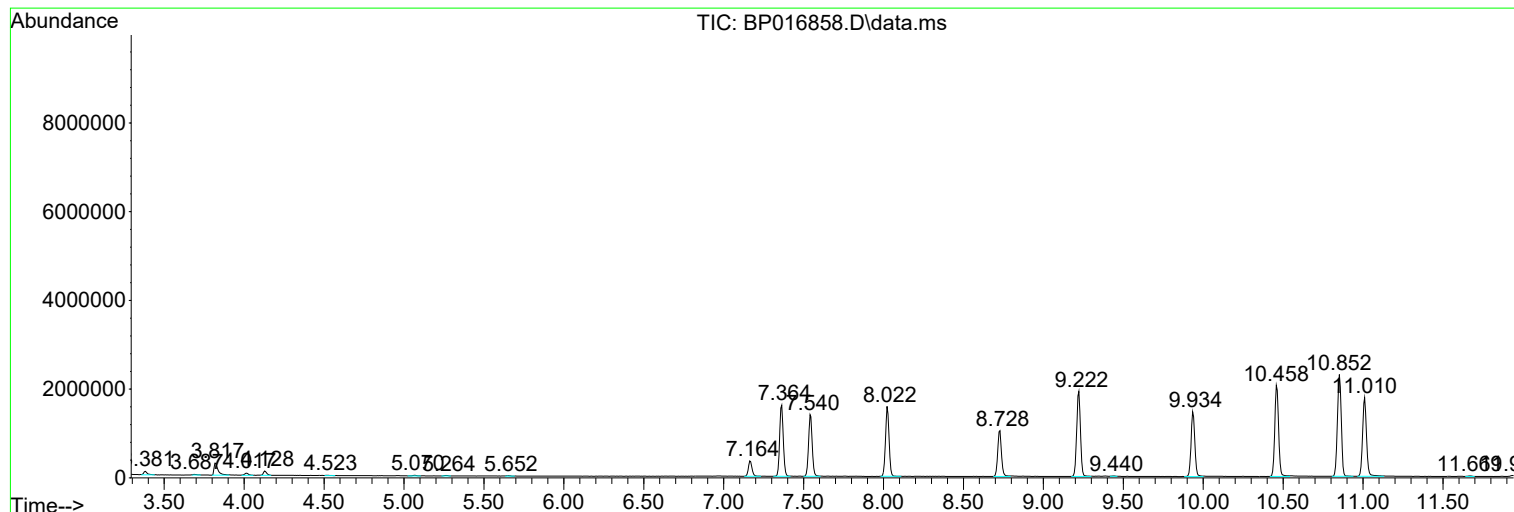

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016858.D
Acq On : 30 Aug 2023 06:24
Operator : MA/JU
Sample : 04159-11
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHL0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016858.D
Acq On : 30 Aug 2023 06:24
Operator : MA/JU
Sample : 04159-11
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHL0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc