

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016860.D
 Acq On : 30 Aug 2023 07:32
 Operator : MA/JU
 Sample : 04159-13
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCHL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016860.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	12	16	23	rVB	82812	113616	0.99%	0.111%
2	3.817	86	90	103	rBV	495361	811201	7.06%	0.789%
3	4.017	118	124	130	rBV	45559	74609	0.65%	0.073%
4	4.128	139	143	154	rVB	94021	145898	1.27%	0.142%
5	5.064	299	302	309	rVB	16136	21206	0.18%	0.021%
6	5.652	397	402	406	rVB3	7037	13469	0.12%	0.013%
7	7.163	653	659	673	rVB	353348	573120	4.99%	0.558%
8	7.358	684	692	706	rBV	1605919	2552882	22.21%	2.484%
9	7.540	717	723	737	rBV	1436429	2281552	19.85%	2.220%
10	8.022	797	805	815	rBV	1501328	2328058	20.25%	2.265%
11	8.728	917	925	936	rBV	1068404	1765348	15.36%	1.718%
12	9.222	1000	1009	1019	rBV	1911091	3146091	27.37%	3.061%
13	9.934	1120	1130	1143	rBV	1479961	2397742	20.86%	2.333%
14	10.457	1211	1219	1231	rBV	2093701	3470538	30.19%	3.377%
15	10.851	1277	1286	1294	rBV	2192213	3592252	31.25%	3.495%
16	11.010	1305	1313	1326	rBV	1898130	3255662	28.32%	3.168%
17	11.669	1421	1425	1430	rVB4	15376	24872	0.22%	0.024%
18	11.928	1464	1469	1477	rVB4	13444	25672	0.22%	0.025%
19	12.428	1548	1554	1562	rVB	44265	82087	0.71%	0.080%
20	13.522	1735	1740	1748	rBV	43086	69417	0.60%	0.068%
21	13.634	1754	1759	1765	rVB4	9299	18450	0.16%	0.018%
22	14.087	1829	1836	1850	rBV	4617017	6255808	54.42%	6.087%
23	14.292	1864	1871	1874	rBV9	5660	12873	0.11%	0.013%
24	14.375	1878	1885	1900	rBV2	5073136	7345275	63.90%	7.147%
25	14.675	1929	1936	1944	rBV	3326169	4827553	42.00%	4.697%
26	14.887	1966	1972	1990	rBV	150420	356884	3.10%	0.347%
27	15.310	2041	2044	2048	rBV6	10967	13877	0.12%	0.014%
28	15.416	2055	2062	2066	rVB5	9302	15530	0.14%	0.015%
29	15.487	2071	2074	2078	rVB4	10612	12263	0.11%	0.012%
30	15.669	2096	2105	2112	rBV	6480256	9659209	84.03%	9.398%
31	15.734	2112	2116	2120	rVV2	119586	208462	1.81%	0.203%
32	15.792	2120	2126	2140	rVV	1713187	2413372	21.00%	2.348%
33	15.910	2142	2146	2159	rVB	38708	76684	0.67%	0.075%
34	16.728	2282	2285	2292	rBV7	7516	14445	0.13%	0.014%
35	17.110	2346	2350	2357	rBV9	10202	19821	0.17%	0.019%
36	17.233	2368	2371	2376	rVB4	9296	12936	0.11%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016860.D
 Acq On : 30 Aug 2023 07:32
 Operator : MA/JU
 Sample : 04159-13
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCHL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

37	17.445	2400	2407	2417	rBV	4029140	5619144	48.88%	5.467%
38	17.545	2417	2424	2437	rBV	7685682	10700221	93.09%	10.411%
39	18.069	2509	2513	2518	rBV7	30361	43689	0.38%	0.043%
40	18.281	2545	2549	2560	rBV2	70508	115732	1.01%	0.113%
41	19.351	2727	2731	2736	rBV2	91434	120113	1.04%	0.117%
42	19.416	2738	2742	2746	rVB	76920	103842	0.90%	0.101%
43	19.516	2756	2759	2765	rBV4	57995	77753	0.68%	0.076%
44	19.780	2798	2804	2815	rBV	8970503	11494922	100.00%	11.185%
45	21.545	3099	3104	3114	rVB	3324560	4414091	38.40%	4.295%
46	23.945	3504	3512	3527	rVB	3809488	8139520	70.81%	7.920%
47	24.110	3534	3540	3553	rVB	1830228	3937612	34.26%	3.831%




Sum of corrected areas: 102775373

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016860.D
Acq On : 30 Aug 2023 07:32
Operator : MA/JU
Sample : 04159-13
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

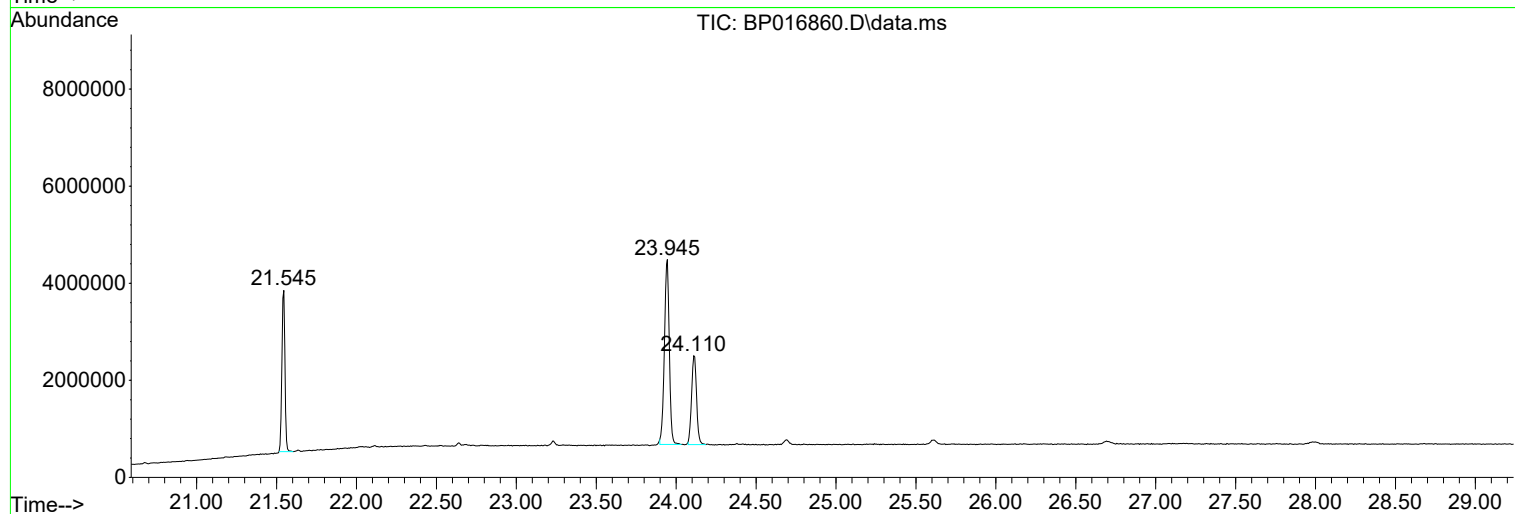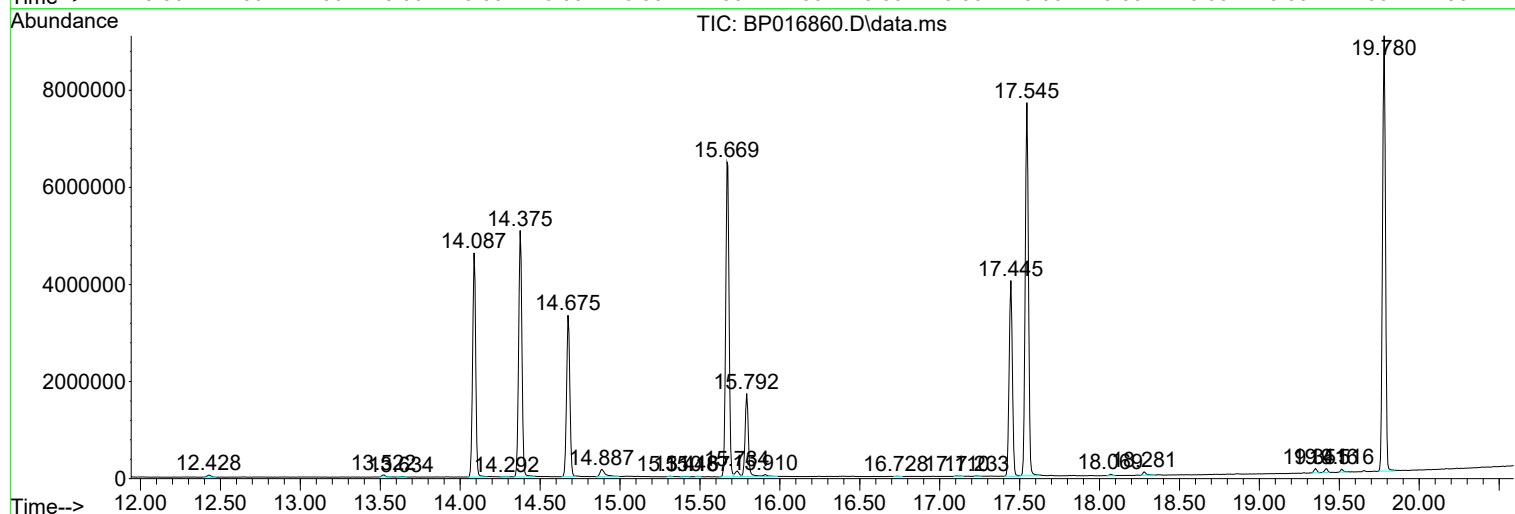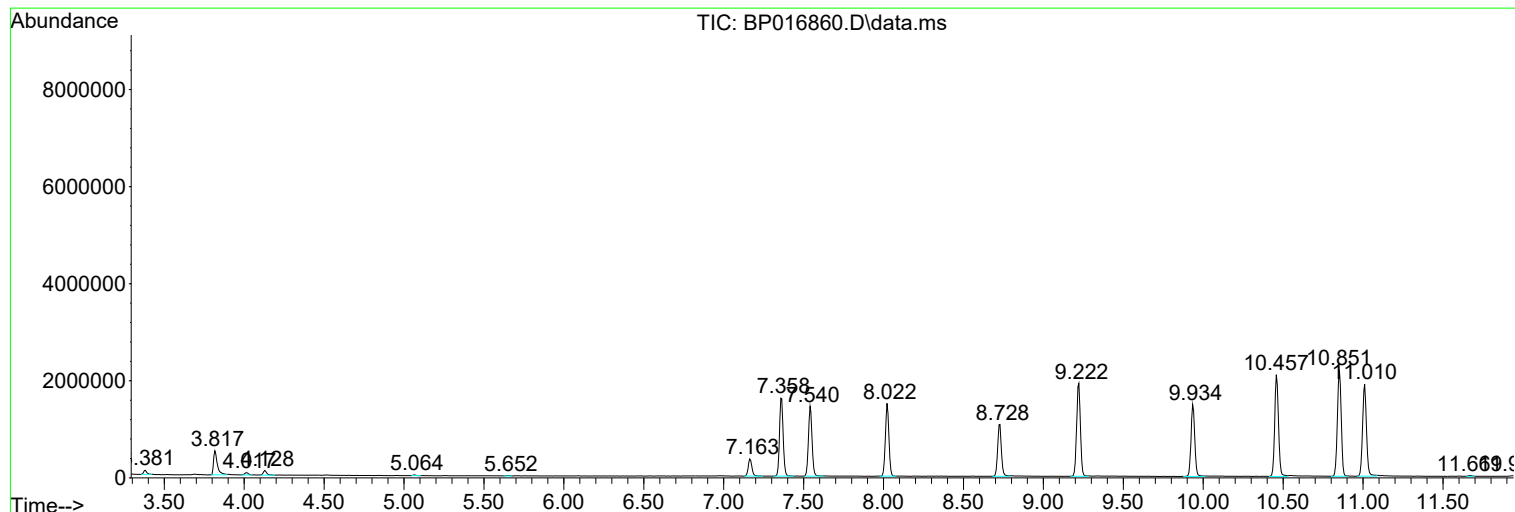

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016860.D
Acq On : 30 Aug 2023 07:32
Operator : MA/JU
Sample : 04159-13
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016860.D
Acq On : 30 Aug 2023 07:32
Operator : MA/JU
Sample : 04159-13
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc