

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016870.D
 Acq On : 30 Aug 2023 13:47
 Operator : MA/JU
 Sample : PB155124BL
 Misc :
 ALS Vial : 90 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK124

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016870.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	12	16	25	rVB	143279	192709	2.02%	0.180%
2	3.811	85	89	115	rBV	1785897	2814725	29.49%	2.626%
3	4.128	139	143	149	rVB	21651	28303	0.30%	0.026%
4	7.164	652	659	674	rBV	2181739	3412612	35.76%	3.184%
5	7.364	685	693	702	rBV	1724324	2716652	28.46%	2.535%
6	7.540	716	723	740	rBV	2153503	3307275	34.65%	3.086%
7	8.022	798	805	816	rBV	1459546	2249754	23.57%	2.099%
8	8.728	917	925	939	rBV	2546628	4166352	43.65%	3.887%
9	9.222	1001	1009	1022	rBV	2028374	3312561	34.71%	3.091%
10	9.934	1120	1130	1145	rBV	1676104	2721110	28.51%	2.539%
11	10.457	1209	1219	1229	rBV	2470094	4092241	42.88%	3.818%
12	10.852	1278	1286	1296	rBV	2044326	3379792	35.41%	3.153%
13	11.010	1303	1313	1340	rBV	2481475	4320456	45.27%	4.031%
14	12.428	1548	1554	1560	rBV	40032	66787	0.70%	0.062%
15	13.516	1734	1739	1744	rBV	28338	45156	0.47%	0.042%
16	13.640	1755	1760	1767	rVB8	9010	17195	0.18%	0.016%
17	14.087	1829	1836	1849	rBV	4451468	5986112	62.72%	5.585%
18	14.375	1878	1885	1905	rBV	5086894	7337493	76.88%	6.846%
19	14.675	1929	1936	1950	rBV	3078661	4444243	46.57%	4.146%
20	14.881	1964	1971	1995	rBV	1463201	2605402	27.30%	2.431%
21	15.669	2098	2105	2119	rBV	6168619	9001042	94.31%	8.398%
22	15.792	2120	2126	2141	rVV	1529623	2086565	21.86%	1.947%
23	15.910	2141	2146	2156	rVB2	31080	62387	0.65%	0.058%
24	17.110	2347	2350	2356	rVB7	9289	13089	0.14%	0.012%
25	17.234	2367	2371	2380	rVB5	7143	13701	0.14%	0.013%
26	17.445	2400	2407	2417	rBV	3644279	5049189	52.90%	4.711%
27	17.545	2417	2424	2443	rVV	6764219	9317601	97.63%	8.693%
28	19.351	2727	2731	2736	rBV2	68922	91786	0.96%	0.086%
29	19.422	2739	2743	2747	rVB	60582	79107	0.83%	0.074%
30	19.781	2798	2804	2819	rBV	7307738	9543970	100.00%	8.904%
31	21.545	3098	3104	3111	rBV	2838283	3907393	40.94%	3.645%
32	23.939	3504	3511	3526	rVB2	3373753	7207308	75.52%	6.724%
33	24.110	3534	3540	3552	rVB	1697991	3594638	37.66%	3.354%


Sum of corrected areas: 107184706

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016870.D
Acq On : 30 Aug 2023 13:47
Operator : MA/JU
Sample : PB155124BL
Misc :
ALS Vial : 90 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK124

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

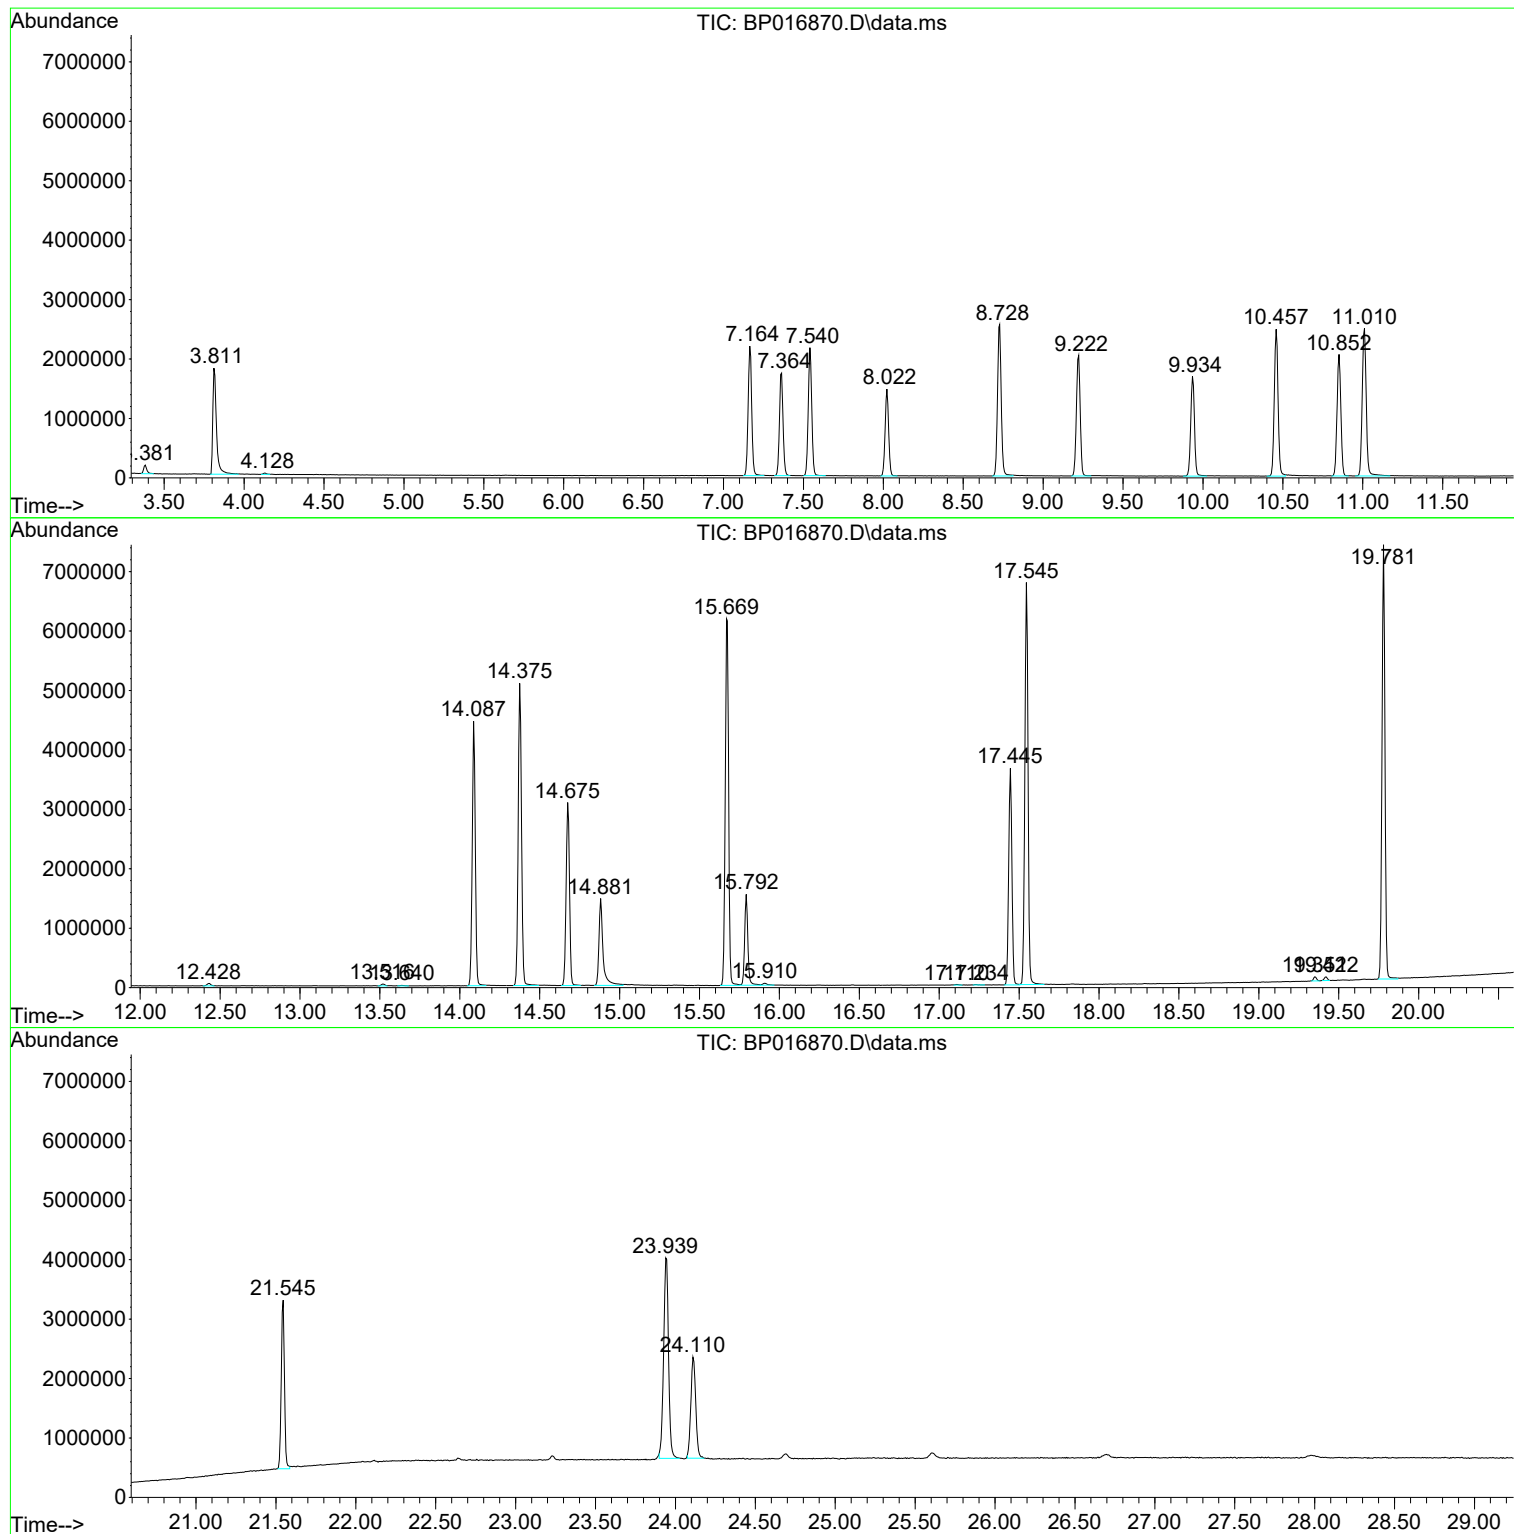

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016870.D
Acq On : 30 Aug 2023 13:47
Operator : MA/JU
Sample : PB155124BL
Misc :
ALS Vial : 90 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK124

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016870.D
Acq On : 30 Aug 2023 13:47
Operator : MA/JU
Sample : PB155124BL
Misc :
ALS Vial : 90 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK124

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc