

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016877.D
 Acq On : 30 Aug 2023 17:48
 Operator : MA/JU
 Sample : 04159-15
 Misc :
 ALS Vial : 96 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCHL5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016877.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	12	16	27	rVB	85769	142663	1.10%	0.130%
2	3.687	65	68	74	rBV5	13573	25095	0.19%	0.023%
3	3.816	87	90	103	rBV	236991	407628	3.15%	0.373%
4	4.011	119	123	135	rVB	51016	95659	0.74%	0.087%
5	4.128	138	143	155	rVB	94758	155564	1.20%	0.142%
6	5.063	299	302	306	rVB	16533	20755	0.16%	0.019%
7	5.258	332	335	340	rBV4	9994	14249	0.11%	0.013%
8	5.652	397	402	406	rBV3	7877	13194	0.10%	0.012%
9	7.163	652	659	671	rBV	424723	676712	5.24%	0.619%
10	7.357	682	692	702	rBV	1741513	2721493	21.05%	2.489%
11	7.540	716	723	734	rBV	1622131	2518192	19.48%	2.303%
12	8.022	798	805	820	rVB	1461233	2300813	17.80%	2.104%
13	8.722	917	924	943	rBV	1224085	1988515	15.38%	1.818%
14	9.222	1000	1009	1025	rBV	2007133	3461186	26.78%	3.165%
15	9.340	1025	1029	1034	rVB7	10165	17169	0.13%	0.016%
16	9.934	1121	1130	1142	rBV	1617655	2607422	20.17%	2.384%
17	10.457	1210	1219	1234	rBV	2285420	3773852	29.19%	3.451%
18	10.851	1277	1286	1300	rBV	2119265	3463938	26.80%	3.168%
19	11.010	1304	1313	1340	rBV	1850965	3242405	25.08%	2.965%
20	12.428	1546	1554	1561	rBV2	43915	71609	0.55%	0.065%
21	13.434	1719	1725	1733	rVB4	16100	29447	0.23%	0.027%
22	13.516	1733	1739	1747	rBV2	36778	68552	0.53%	0.063%
23	13.634	1752	1759	1763	rBV5	8844	14605	0.11%	0.013%
24	14.086	1829	1836	1849	rBV	4541840	6261252	48.44%	5.726%
25	14.375	1878	1885	1903	rBV2	5257753	7625544	58.99%	6.973%
26	14.504	1904	1907	1912	rVB6	9157	14081	0.11%	0.013%
27	14.675	1929	1936	1944	rBV	3152426	4583752	35.46%	4.192%
28	14.886	1965	1972	1989	rBV	195430	450033	3.48%	0.412%
29	15.110	2007	2010	2017	rVB9	12514	18828	0.15%	0.017%
30	15.416	2058	2062	2066	rVB	13244	17511	0.14%	0.016%
31	15.457	2066	2069	2077	rBV4	17232	31108	0.24%	0.028%
32	15.675	2096	2106	2113	rBV	6648908	9764180	75.54%	8.929%
33	15.792	2120	2126	2134	rBV	1848656	2436570	18.85%	2.228%
34	15.910	2142	2146	2150	rVB	29435	36882	0.29%	0.034%
35	16.333	2212	2218	2223	rBV2	41756	82545	0.64%	0.075%
36	17.127	2350	2353	2356	rVB	32533	36266	0.28%	0.033%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016877.D
 Acq On : 30 Aug 2023 17:48
 Operator : MA/JU
 Sample : 04159-15
 Misc :
 ALS Vial : 96 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCHL5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

37	17.169	2356	2360	2365	rVB2	32641	44238	0.34%	0.040%
38	17.445	2400	2407	2417	rBV	3906253	5585011	43.21%	5.107%
39	17.545	2417	2424	2441	rVV	8002921	11228199	86.86%	10.268%
40	17.874	2476	2480	2484	rVB	40554	51485	0.40%	0.047%
41	18.063	2508	2512	2518	rVB3	45253	64601	0.50%	0.059%
42	18.280	2545	2549	2557	rBV	171981	270731	2.09%	0.248%
43	18.369	2561	2564	2568	rVV2	23190	31450	0.24%	0.029%
44	18.545	2591	2594	2597	rBV2	38470	41766	0.32%	0.038%
45	19.157	2695	2698	2702	rVB	31446	30988	0.24%	0.028%
46	19.198	2702	2705	2708	rBV4	22181	28646	0.22%	0.026%
47	19.351	2727	2731	2735	rVB2	98651	118414	0.92%	0.108%
48	19.416	2739	2742	2748	rVB	90768	124979	0.97%	0.114%
49	19.516	2755	2759	2765	rBV2	94502	133342	1.03%	0.122%
50	19.780	2798	2804	2814	rBV	10110152	12926388	100.00%	11.821%
51	21.539	3098	3103	3112	rBV2	3760433	4979277	38.52%	4.553%
52	23.939	3502	3511	3530	rVB2	4808662	10144238	78.48%	9.277%
53	24.109	3533	3540	3550	rVB	2029798	4358593	33.72%	3.986%




Sum of corrected areas: 109351615

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016877.D
Acq On : 30 Aug 2023 17:48
Operator : MA/JU
Sample : 04159-15
Misc :
ALS Vial : 96 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHL5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

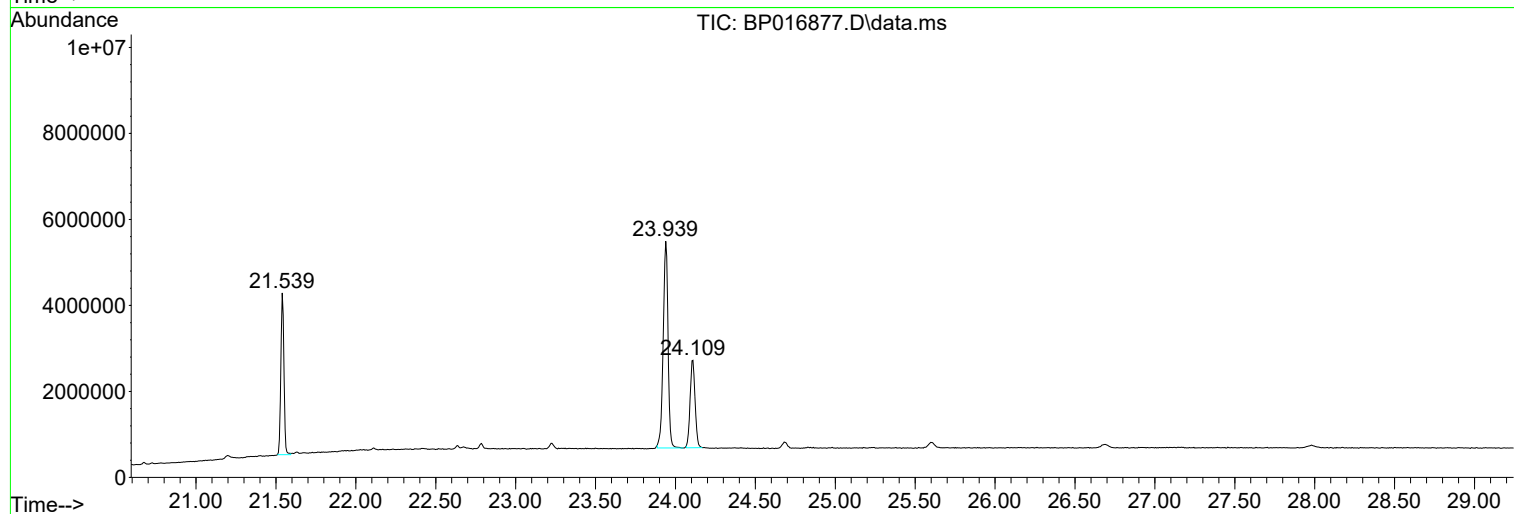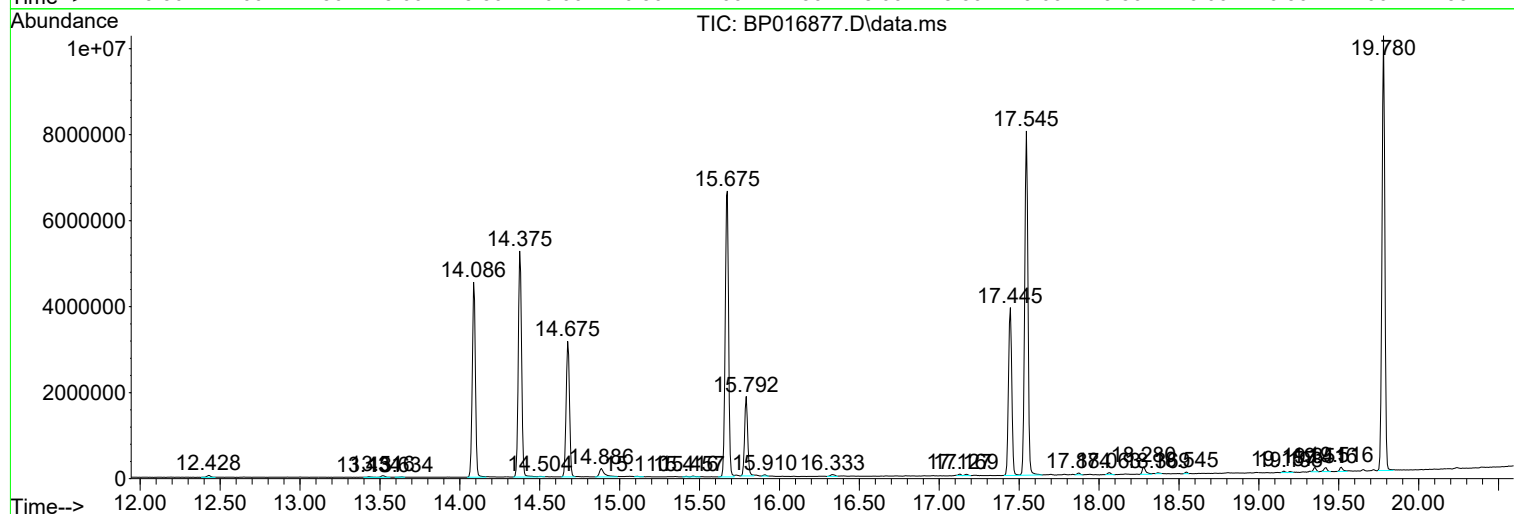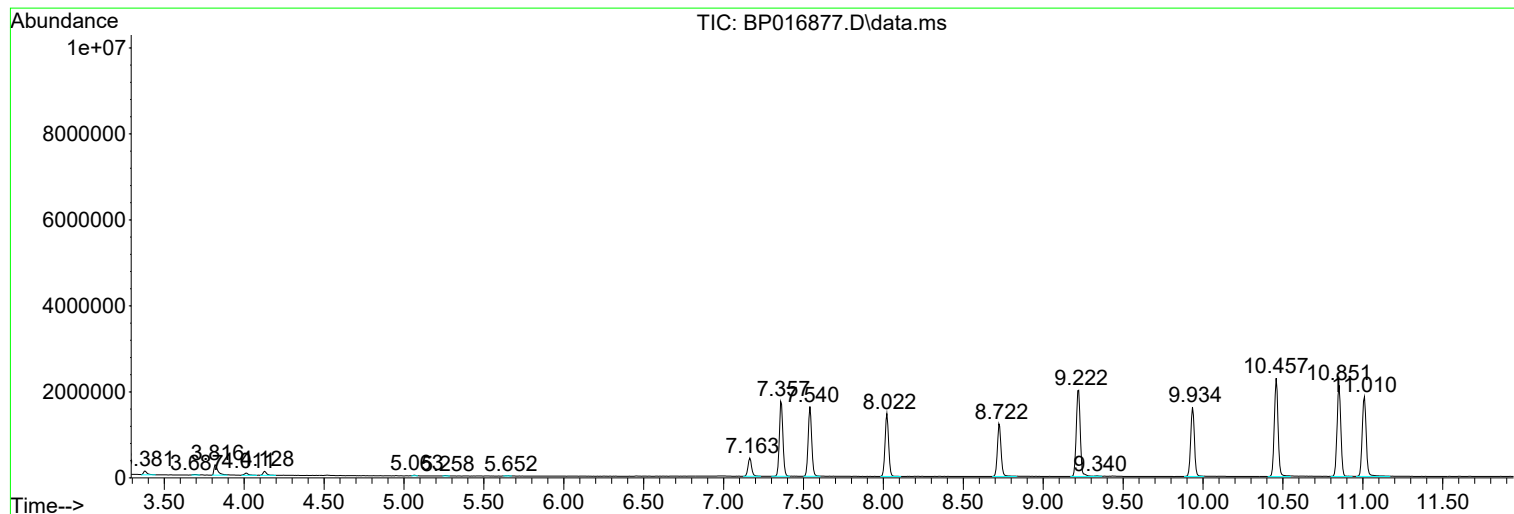

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016877.D
Acq On : 30 Aug 2023 17:48
Operator : MA/JU
Sample : 04159-15
Misc :
ALS Vial : 96 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHL5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016877.D
Acq On : 30 Aug 2023 17:48
Operator : MA/JU
Sample : 04159-15
Misc :
ALS Vial : 96 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHL5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------