

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016878.D
 Acq On : 30 Aug 2023 19:04
 Operator : MA/JU
 Sample : 04159-16
 Misc :
 ALS Vial : 97 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCHL6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016878.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	11	15	26	rVB	97429	176399	1.48%	0.170%
2	3.811	85	89	104	rBV	491915	825090	6.93%	0.794%
3	4.011	118	123	131	rVB	47091	78732	0.66%	0.076%
4	4.122	137	142	153	rVB	92565	138730	1.17%	0.133%
5	5.058	297	301	307	rVB	18385	28510	0.24%	0.027%
6	5.646	398	401	405	rVB4	10237	14389	0.12%	0.014%
7	7.158	652	658	669	rBV	428716	677998	5.70%	0.652%
8	7.358	685	692	701	rBV	1542999	2456424	20.63%	2.364%
9	7.534	715	722	734	rBV	1477765	2355443	19.79%	2.266%
10	8.016	797	804	815	rBV	1387141	2207020	18.54%	2.124%
11	8.546	891	894	901	rVB4	10520	18037	0.15%	0.017%
12	8.722	913	924	939	rBV	1198611	1954288	16.42%	1.880%
13	8.893	948	953	958	rVB2	20458	35084	0.29%	0.034%
14	9.134	989	994	998	rBV6	11621	19606	0.16%	0.019%
15	9.216	1000	1008	1021	rVV	1920365	3088436	25.94%	2.972%
16	9.334	1023	1028	1032	rVB8	8809	15153	0.13%	0.015%
17	9.434	1042	1045	1051	rVB4	15255	23053	0.19%	0.022%
18	9.934	1118	1130	1142	rBV	1444980	2421867	20.34%	2.330%
19	10.252	1178	1184	1189	rVB7	12982	25568	0.21%	0.025%
20	10.457	1207	1219	1227	rBV	2099753	3499338	29.39%	3.367%
21	10.699	1255	1260	1266	rVB5	15282	28644	0.24%	0.028%
22	10.846	1277	1285	1293	rBV	1978797	3340305	28.06%	3.214%
23	10.910	1293	1296	1301	rVB7	12686	18641	0.16%	0.018%
24	11.004	1305	1312	1327	rBV2	1791283	3371708	28.32%	3.244%
25	11.240	1345	1352	1357	rVB8	16383	33415	0.28%	0.032%
26	11.446	1381	1387	1395	rVB2	34046	56794	0.48%	0.055%
27	11.675	1420	1426	1429	rBV8	9354	16377	0.14%	0.016%
28	11.934	1465	1470	1474	rVB4	17016	26232	0.22%	0.025%
29	12.010	1479	1483	1487	rVB4	11893	19025	0.16%	0.018%
30	12.428	1547	1554	1562	rVB3	42021	79835	0.67%	0.077%
31	12.528	1562	1571	1575	rBV3	6087	16437	0.14%	0.016%
32	12.693	1596	1599	1604	rVV7	9231	19668	0.17%	0.019%
33	12.740	1604	1607	1613	rVB8	11387	19093	0.16%	0.018%
34	12.810	1613	1619	1622	rBV4	26052	39564	0.33%	0.038%
35	12.857	1622	1627	1637	rVB8	27589	65157	0.55%	0.063%
36	13.369	1708	1714	1722	rBV10	10094	32463	0.27%	0.031%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016878.D
 Acq On : 30 Aug 2023 19:04
 Operator : MA/JU
 Sample : 04159-16
 Misc :
 ALS Vial : 97 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCHL6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

37	13.434	1722	1725	1727	rVV3	12902	16175	0.14%	0.016%
38	13.457	1727	1729	1734	rVV6	9476	13376	0.11%	0.013%
39	13.516	1734	1739	1745	rVB3	23474	42267	0.36%	0.041%
40	13.628	1756	1758	1764	rVB5	7730	12340	0.10%	0.012%

41	13.693	1764	1769	1774	rBV3	18549	34017	0.29%	0.033%
42	13.828	1787	1792	1797	rBV9	11427	18276	0.15%	0.018%
43	13.910	1805	1806	1811	rVB5	9926	12829	0.11%	0.012%
44	14.087	1827	1836	1849	rBV	4258561	5843029	49.08%	5.622%
45	14.222	1855	1859	1865	rVB8	13792	25121	0.21%	0.024%

46	14.375	1878	1885	1903	rBV	4801615	6962956	58.49%	6.700%
47	14.675	1930	1936	1951	rVB	2991003	4433247	37.24%	4.266%
48	14.828	1958	1962	1966	rVB2	17623	26239	0.22%	0.025%
49	14.887	1966	1972	1981	rBV	235048	444786	3.74%	0.428%
50	15.210	2019	2027	2037	rBV	85808	144857	1.22%	0.139%

51	15.292	2037	2041	2044	rBV4	27489	44536	0.37%	0.043%
52	15.410	2058	2061	2068	rVB6	16118	26828	0.23%	0.026%
53	15.481	2068	2073	2079	rVB6	14427	25859	0.22%	0.025%
54	15.675	2096	2106	2112	rBV	6432716	9142350	76.79%	8.797%
55	15.734	2112	2116	2121	rVV	180559	306211	2.57%	0.295%

56	15.792	2121	2126	2141	rVV	1913149	2722403	22.87%	2.619%
57	15.916	2142	2147	2154	rVB4	85017	148538	1.25%	0.143%
58	16.022	2164	2165	2171	rVB6	10686	15349	0.13%	0.015%
59	16.257	2200	2205	2208	rBV6	13318	19964	0.17%	0.019%
60	16.451	2233	2238	2244	rVB3	22487	42479	0.36%	0.041%

61	17.004	2330	2332	2338	rVB7	12049	16083	0.14%	0.015%
62	17.069	2338	2343	2347	rBV	74669	109775	0.92%	0.106%
63	17.239	2367	2372	2374	rBV6	10052	17558	0.15%	0.017%
64	17.445	2401	2407	2418	rBV	3752889	5288363	44.42%	5.088%
65	17.551	2418	2425	2439	rBV	7013742	10301772	86.53%	9.912%

66	17.657	2441	2443	2447	rBV5	11329	19421	0.16%	0.019%
67	17.810	2465	2469	2472	rBV2	34982	49117	0.41%	0.047%
68	17.951	2489	2493	2496	rBV6	9598	14310	0.12%	0.014%
69	18.075	2510	2514	2517	rBV5	34514	45616	0.38%	0.044%
70	18.157	2524	2528	2535	rBV7	21430	42308	0.36%	0.041%

71	18.281	2546	2549	2559	rBV	134225	201586	1.69%	0.194%
72	18.416	2570	2572	2576	rVB3	16438	17766	0.15%	0.017%
73	19.351	2727	2731	2736	rVB3	84953	112167	0.94%	0.108%
74	19.422	2740	2743	2748	rVB	93749	111002	0.93%	0.107%
75	19.516	2756	2759	2764	rBV5	74855	100234	0.84%	0.096%

76	19.657	2780	2783	2786	rBV2	31967	38554	0.32%	0.037%
----	--------	------	------	------	------	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016878.D
Acq On : 30 Aug 2023 19:04
Operator : MA/JU
Sample : 04159-16
Misc :
ALS Vial : 97 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHL6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Title : SVOA CALIBRATION

77	19.780	2798	2804	2817	rBV	9052831	11904992	100.00%	11.455%
78	21.545	3099	3104	3111	rBV	3681575	4751574	39.91%	4.572%
79	23.945	3503	3512	3525	rVB2	4251931	9015876	75.73%	8.675%
80	24.115	3534	3541	3550	rVB	1899716	4005681	33.65%	3.854%




Sum of corrected areas: 103930310

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016878.D
Acq On : 30 Aug 2023 19:04
Operator : MA/JU
Sample : 04159-16
Misc :
ALS Vial : 97 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHL6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

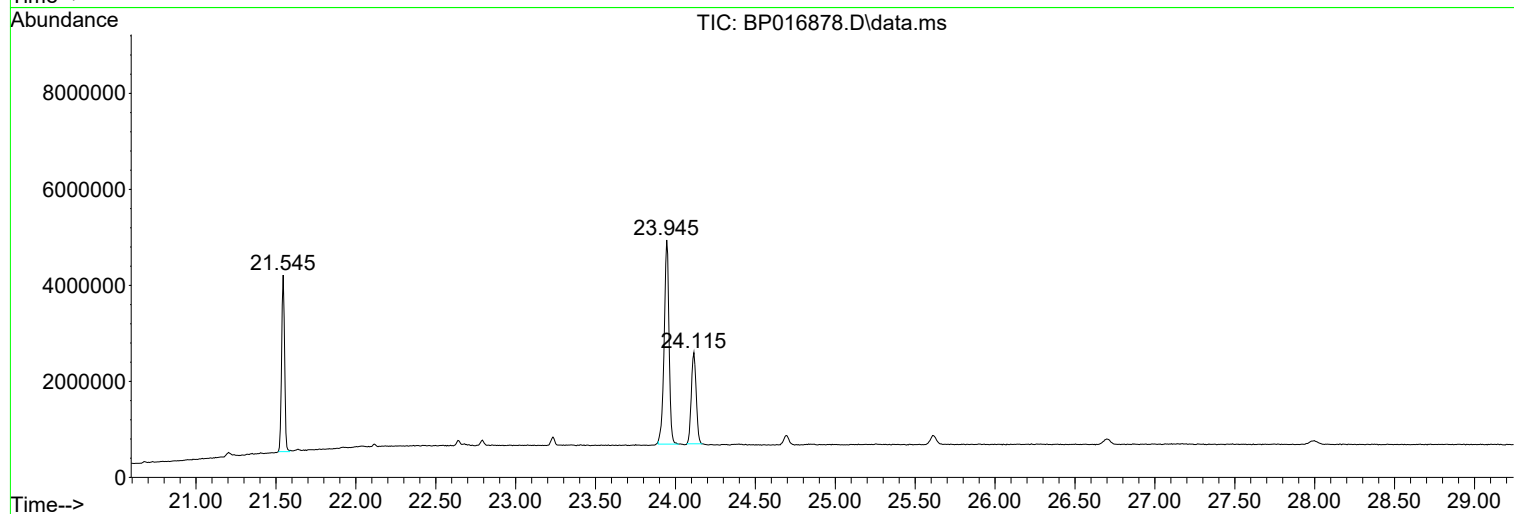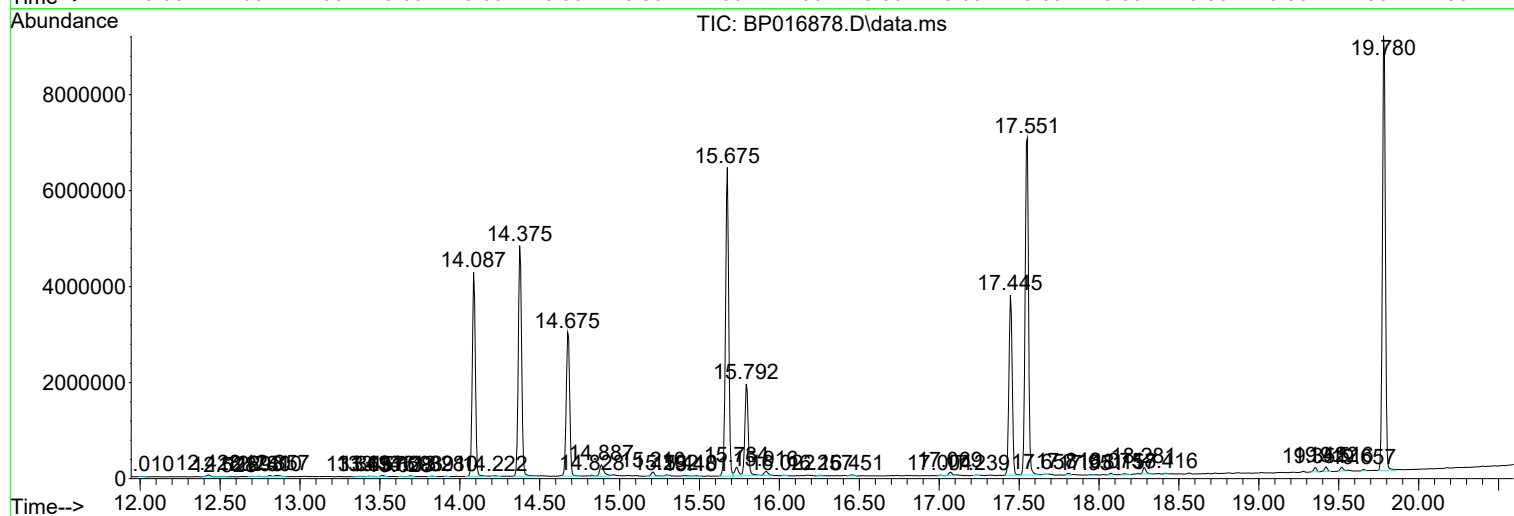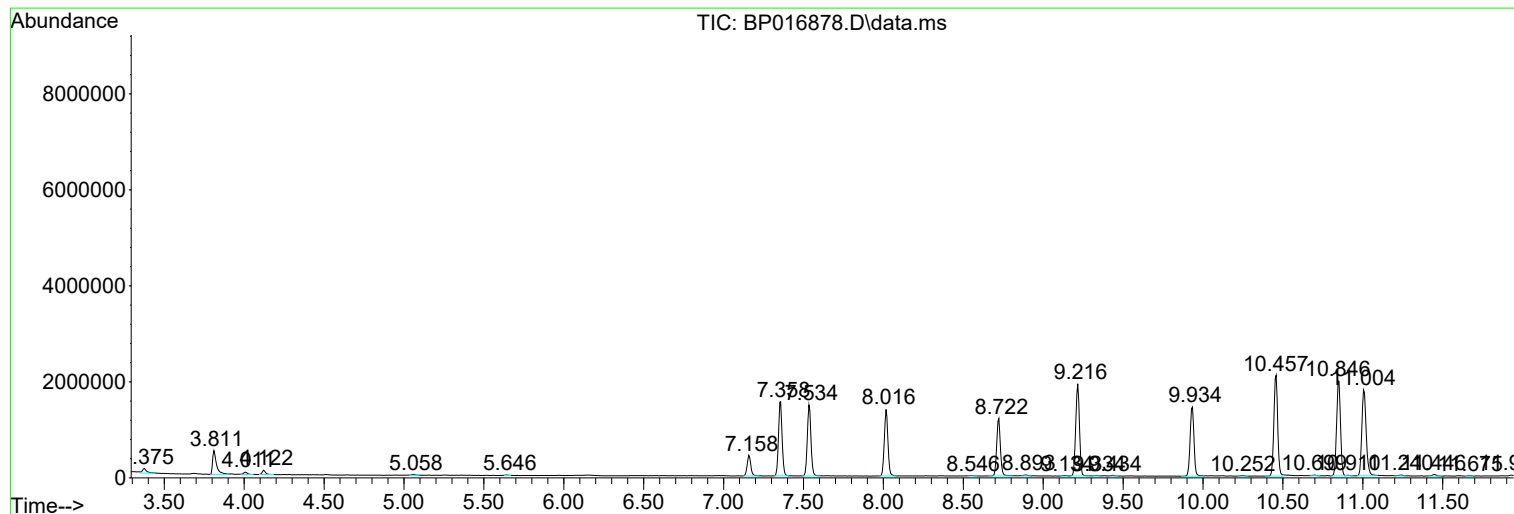

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016878.D
Acq On : 30 Aug 2023 19:04
Operator : MA/JU
Sample : 04159-16
Misc :
ALS Vial : 97 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHL6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016878.D
Acq On : 30 Aug 2023 19:04
Operator : MA/JU
Sample : 04159-16
Misc :
ALS Vial : 97 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHL6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------