

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016881.D
 Acq On : 30 Aug 2023 20:47
 Operator : MA/JU
 Sample : PB155126BL
 Misc :
 ALS Vial : 100 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK126

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016881.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	11	15	26	rVB	122079	180791	1.69%	0.151%
2	3.811	85	89	113	rBV	1665164	2715220	25.33%	2.262%
3	4.128	139	143	151	rVB	42209	62658	0.58%	0.052%
4	6.463	536	540	546	rBV7	6227	11932	0.11%	0.010%
5	7.163	652	659	677	rBV	2115877	3307239	30.86%	2.755%
6	7.357	684	692	702	rBV	1682579	2605987	24.32%	2.171%
7	7.540	715	723	736	rBV	2042033	3194638	29.81%	2.662%
8	8.022	797	805	814	rBV	1909498	2982771	27.83%	2.485%
9	8.722	917	924	938	rBV	2528437	4098787	38.24%	3.415%
10	9.216	998	1008	1024	rBV	1979600	3254908	30.37%	2.712%
11	9.934	1120	1130	1141	rBV	1658337	2655990	24.78%	2.213%
12	10.457	1211	1219	1230	rBV	2501691	4087171	38.14%	3.405%
13	10.851	1278	1286	1299	rVB	2781977	4607537	42.99%	3.839%
14	11.010	1304	1313	1335	rBV	2459695	4257774	39.73%	3.547%
15	12.428	1549	1554	1561	rVB2	43239	72969	0.68%	0.061%
16	12.645	1585	1591	1595	rBV9	6218	13461	0.13%	0.011%
17	13.522	1733	1740	1745	rBV4	14860	25238	0.24%	0.021%
18	14.087	1830	1836	1848	rBV	4415816	5951001	55.53%	4.958%
19	14.375	1877	1885	1901	rBV	5153294	7380726	68.87%	6.149%
20	14.675	1929	1936	1952	rBV	4286367	6311611	58.89%	5.259%
21	14.798	1952	1957	1964	rVB	5438	13030	0.12%	0.011%
22	14.881	1964	1971	1991	rBV	1570495	2782503	25.96%	2.318%
23	15.069	2001	2003	2008	rVB6	9633	12965	0.12%	0.011%
24	15.669	2098	2105	2120	rBV	6364232	9112990	85.03%	7.593%
25	15.792	2120	2126	2139	rVV	1658523	2298637	21.45%	1.915%
26	15.904	2142	2145	2155	rVB2	31007	53619	0.50%	0.045%
27	17.104	2346	2349	2354	rBV7	8088	11898	0.11%	0.010%
28	17.228	2367	2370	2375	rVB2	9995	12065	0.11%	0.010%
29	17.445	2400	2407	2417	rBV	5530004	7545741	70.41%	6.287%
30	17.545	2417	2424	2445	rVB2	7042278	9835974	91.77%	8.195%
31	18.280	2546	2549	2557	rBV7	22853	35872	0.33%	0.030%
32	19.351	2727	2731	2735	rBV	80229	106461	0.99%	0.089%
33	19.416	2739	2742	2747	rVB2	66398	91842	0.86%	0.077%
34	19.780	2798	2804	2815	rBV	8246442	10717556	100.00%	8.929%
35	21.545	3098	3104	3114	rBV	4702452	6443741	60.12%	5.369%
36	23.939	3503	3511	3529	rVB2	3579268	7738322	72.20%	6.447%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016881.D
Acq On : 30 Aug 2023 20:47
Operator : MA/JU
Sample : PB155126BL
Misc :
ALS Vial : 100 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK126

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Title : SVOA CALIBRATION

37	24.110	3533	3540	3551	rVB	2522371	5433872	50.70%	4.527%
----	--------	------	------	------	-----	---------	---------	--------	--------


Sum of corrected areas: 120025497

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016881.D
Acq On : 30 Aug 2023 20:47
Operator : MA/JU
Sample : PB155126BL
Misc :
ALS Vial : 100 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK126

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

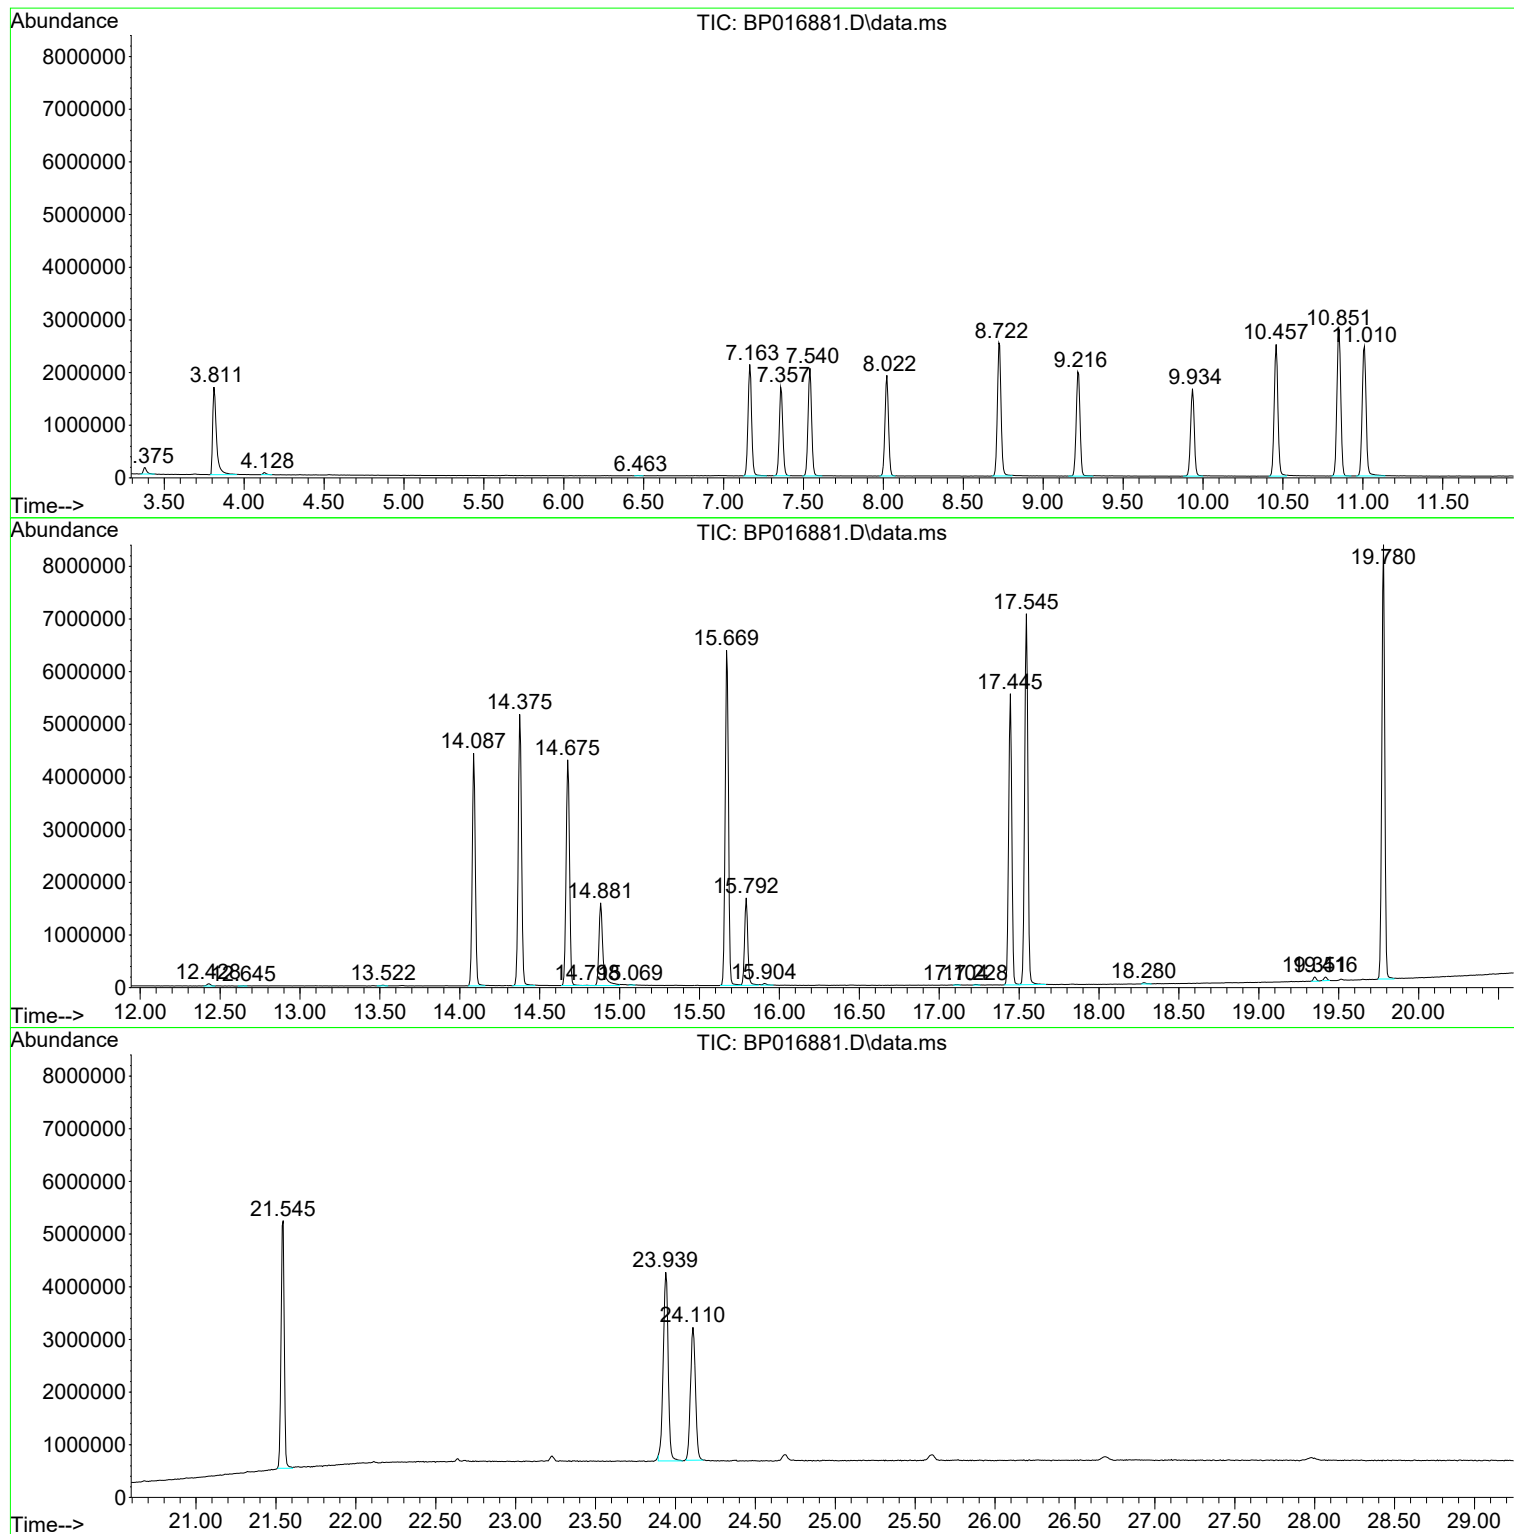

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016881.D
Acq On : 30 Aug 2023 20:47
Operator : MA/JU
Sample : PB155126BL
Misc :
ALS Vial : 100 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK126

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016881.D
Acq On : 30 Aug 2023 20:47
Operator : MA/JU
Sample : PB155126BL
Misc :
ALS Vial : 100 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK126

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------