

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082825\
 Data File : BP025611.D
 Acq On : 28 Aug 2025 14:28
 Operator : CG/JU
 Sample : PB169431BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB169431BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP025611.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.931	334	339	349	rBV	431336	623781	5.27%	1.288%
2	5.402	411	419	435	rBV	2953625	4486398	37.88%	9.264%
3	6.960	674	684	700	rBV	2527688	4398079	37.13%	9.081%
4	7.772	815	822	836	rVB	593647	989489	8.35%	2.043%
5	8.913	1007	1016	1029	rBV	1641035	2957827	24.97%	6.107%
6	10.542	1283	1293	1309	rBV	721977	1324213	11.18%	2.734%
7	12.995	1703	1710	1728	rBV	4322820	6473903	54.65%	13.367%
8	14.389	1940	1947	1955	rBV	1003615	1693538	14.30%	3.497%
9	15.907	2195	2205	2220	rBV	3340210	5482349	46.28%	11.320%
10	17.189	2416	2423	2438	rBV	1253089	2215334	18.70%	4.574%
11	19.907	2879	2885	2899	rBV	8614479	11845126	100.00%	24.458%
12	20.848	3042	3045	3051	rBV3	70093	151207	1.28%	0.312%
13	21.642	3173	3180	3193	rVB2	1357935	2866183	24.20%	5.918%
14	25.012	3743	3753	3771	rVB	873531	2923086	24.68%	6.036%




Sum of corrected areas: 48430513

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082825\
Data File : BP025611.D
Acq On : 28 Aug 2025 14:28
Operator : CG/JU
Sample : PB169431BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB169431BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

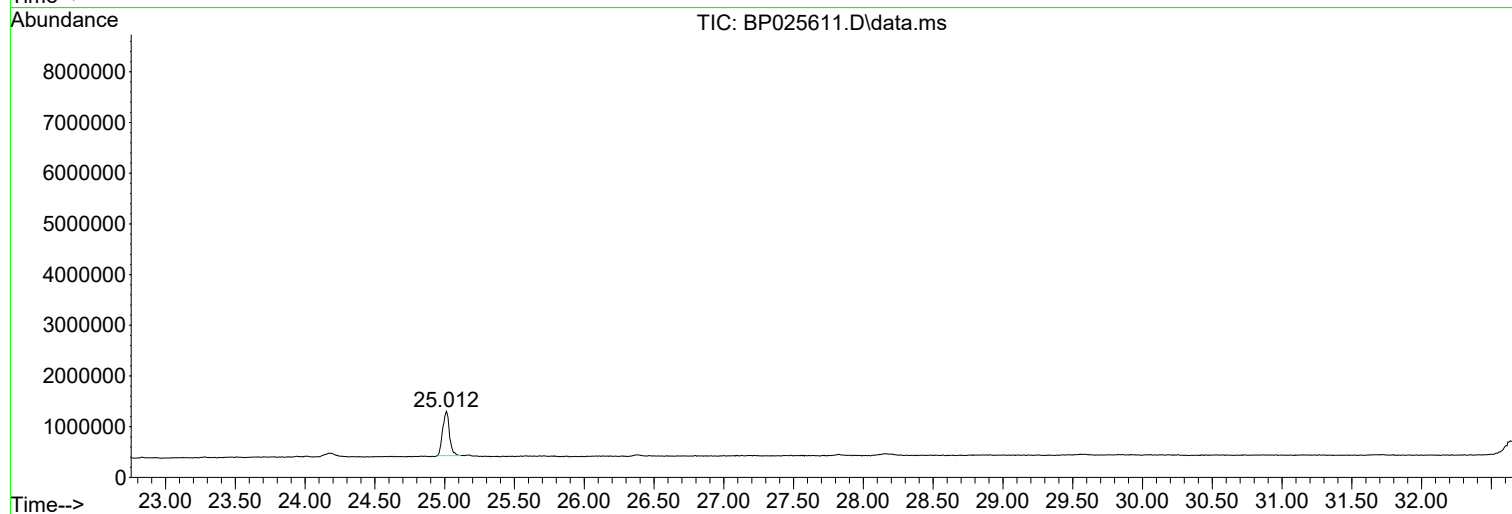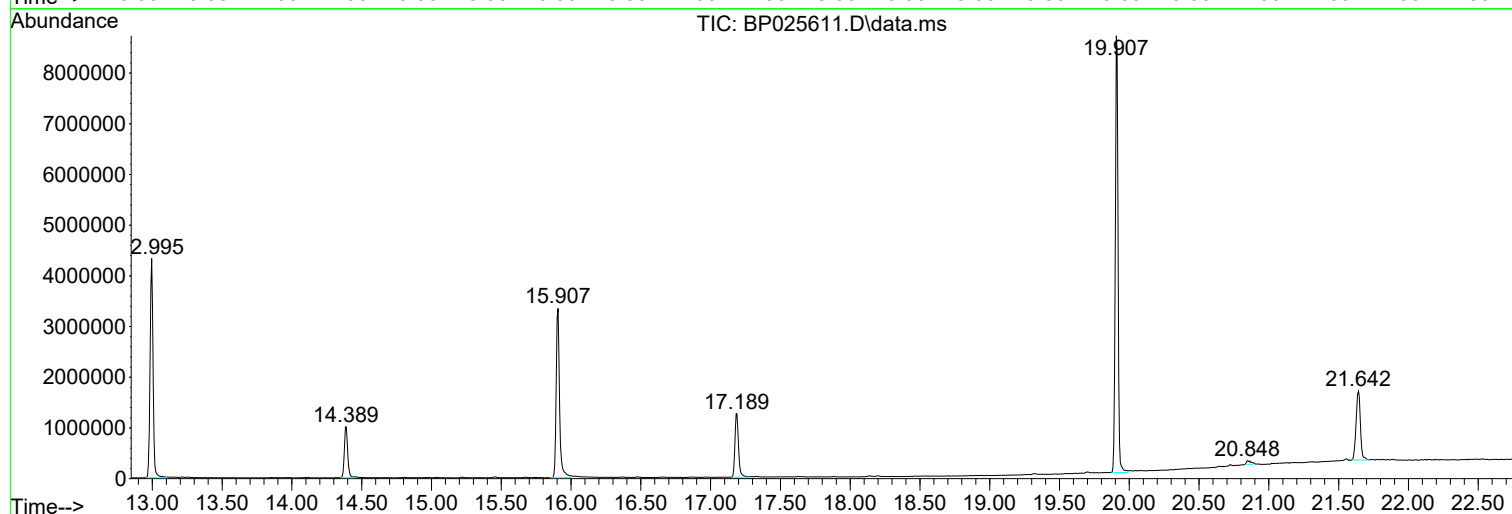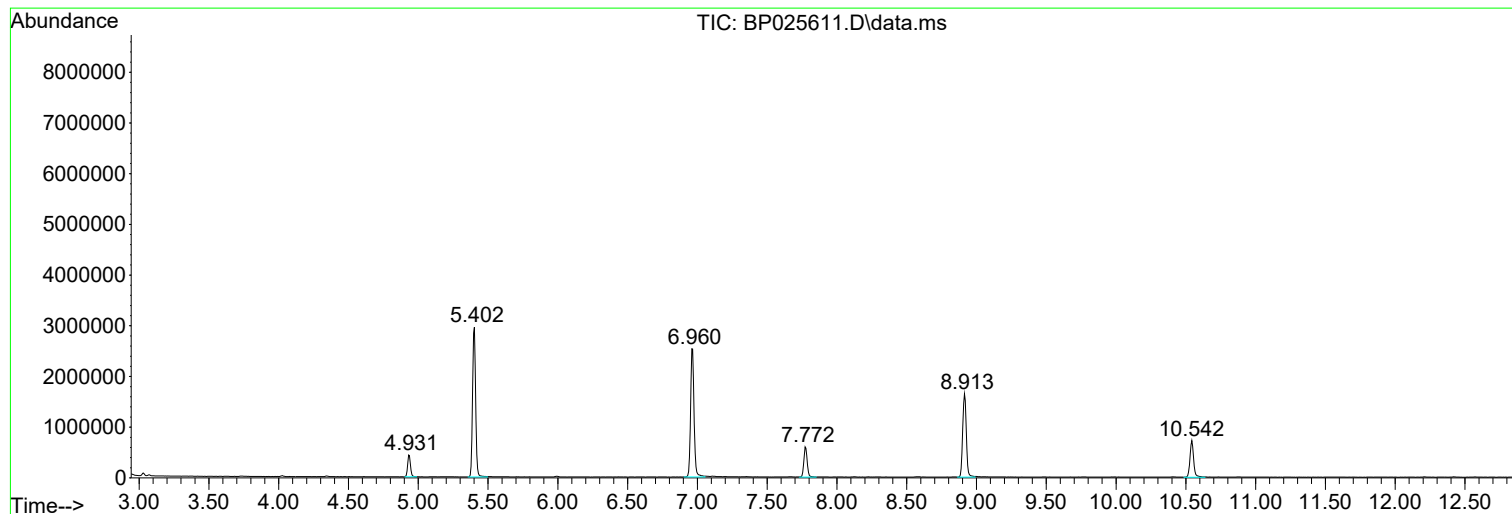

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082825\
Data File : BP025611.D
Acq On : 28 Aug 2025 14:28
Operator : CG/JU
Sample : PB169431BL
Misc :
ALS Vial : 3 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
PB169431BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD			R.T.
4.931	12.61 ng	623781	1,4-Dichlorobenzene-d4			7.772
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-		116	C6H12O2	000123-42-2	56
2	Acetic acid, cyano-, 1,1-dimethy...		141	C7H11NO2	001116-98-9	17
3	1-Propen-2-ol, acetate		100	C5H8O2	000108-22-5	10
4	Butane, 1-ethoxy-		102	C6H14O	000628-81-9	9
5	Morpholine, 4-methyl-		101	C5H11NO	000109-02-4	9

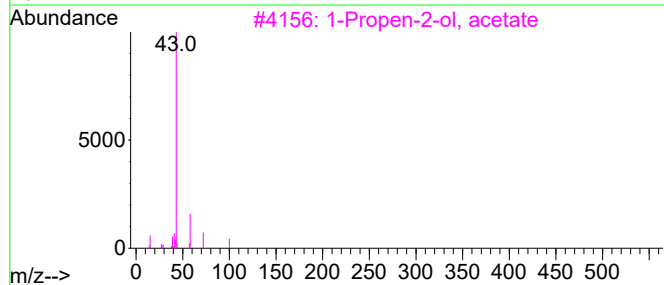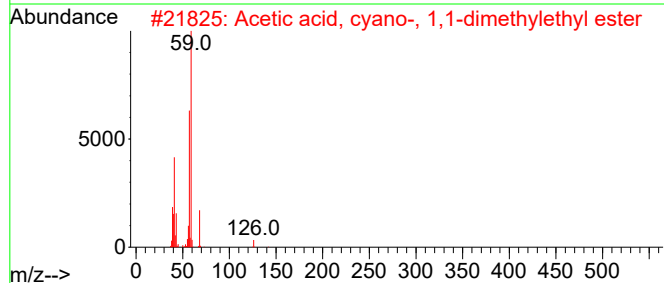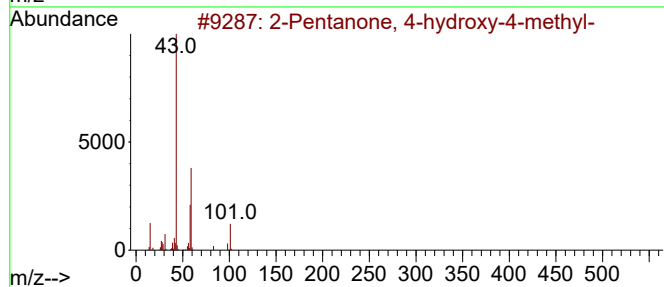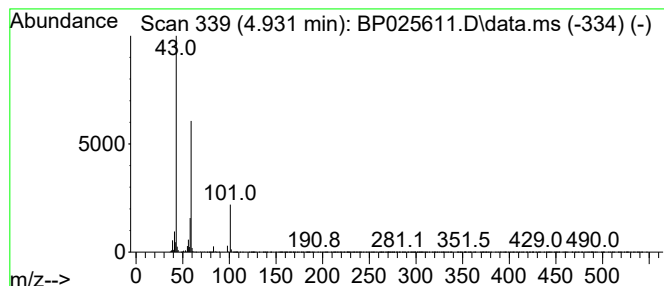

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082825\
Data File : BP025611.D
Acq On : 28 Aug 2025 14:28
Operator : CG/JU
Sample : PB169431BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB169431BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.931	12.6	ng	623781	1	7.772	989489	20.0