


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082825\
Data File : BP025609.D
Acq On : 28 Aug 2025 13:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 14 18:14:31 2025

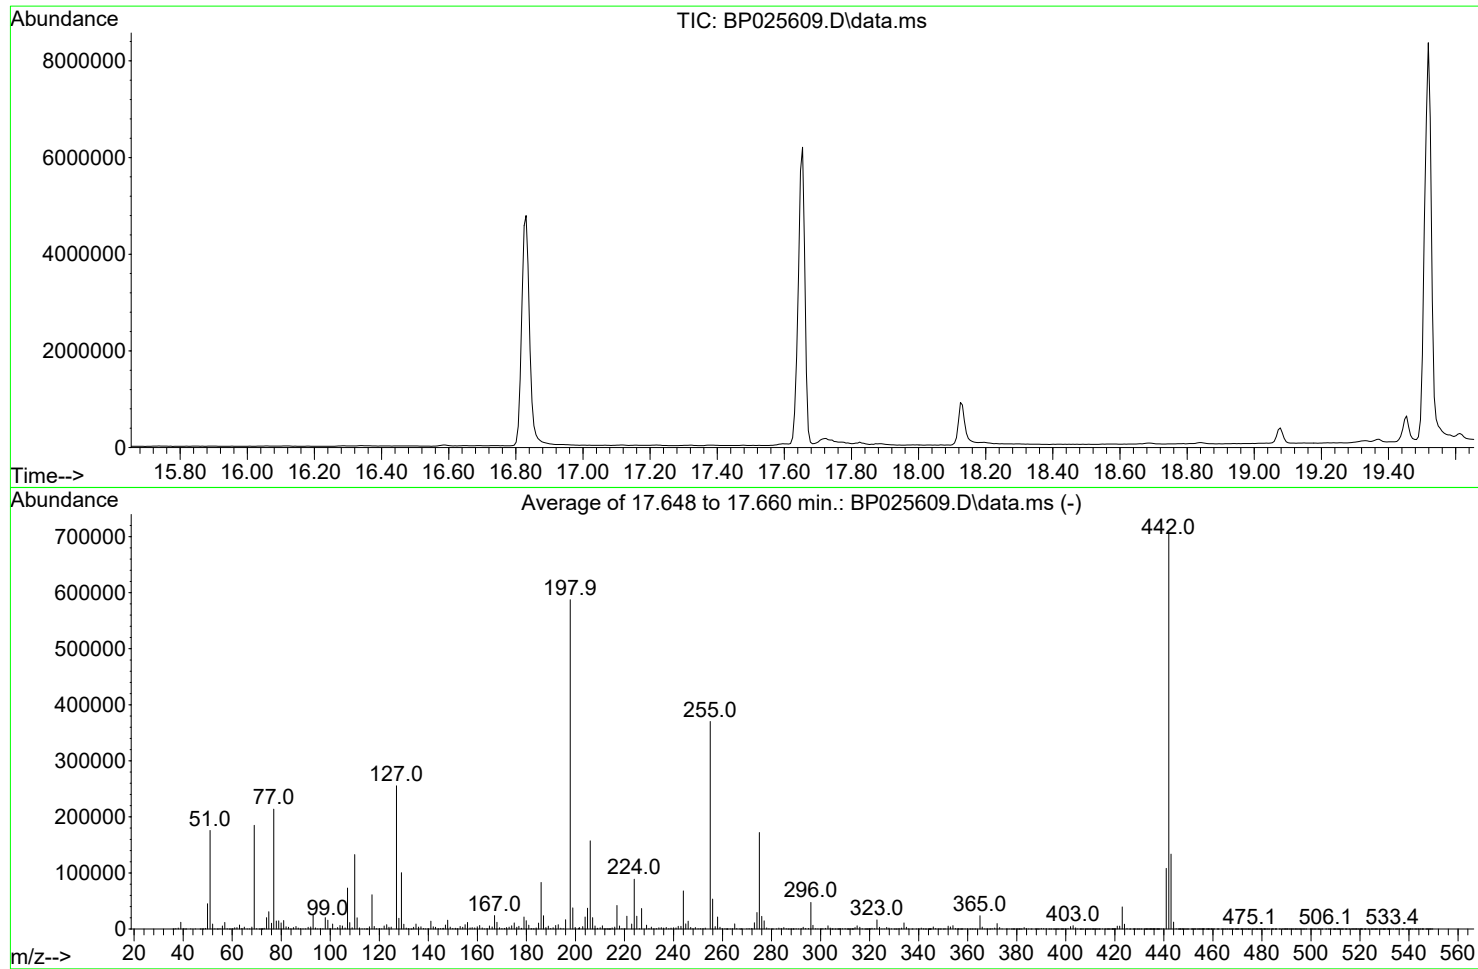

AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2492

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.8	3346	PASS
69	69	100	100	100.0	184973	PASS
70	69	0.00	2	0.4	716	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	587623	PASS
199	198	5	9	6.4	37813	PASS
365	198	1	100	4.0	23656	PASS
441	443	0.01	150	81.0	108302	PASS
442	442	100	100	100.0	704405	PASS
443	442	15	24	19.0	133753	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/28/2025	BNA_P	<u>BP025609.D</u>
Compound Name	Response	Retention Time
DDT	2563922	20.813
DDD	52854	20.348
DDE	7833	19.819
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
60687	2624609	2.31

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082825\
Data File : BP025609.D
Acq On : 28 Aug 2025 13:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 28 15:31:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

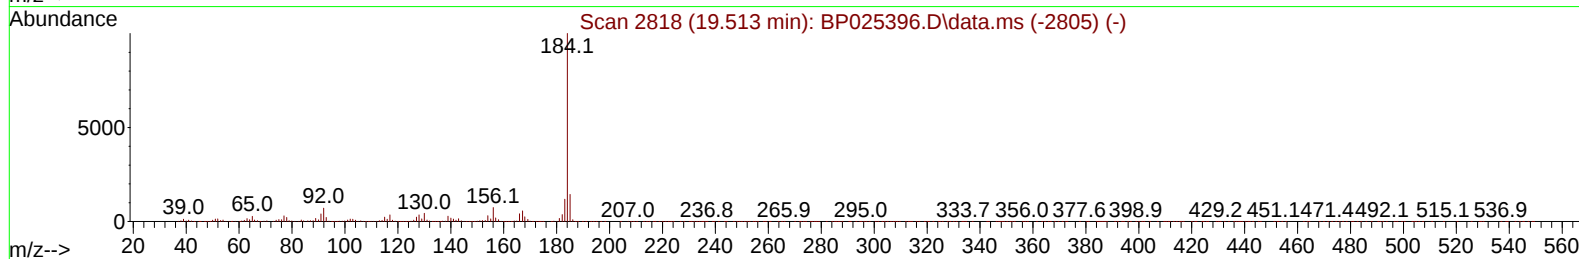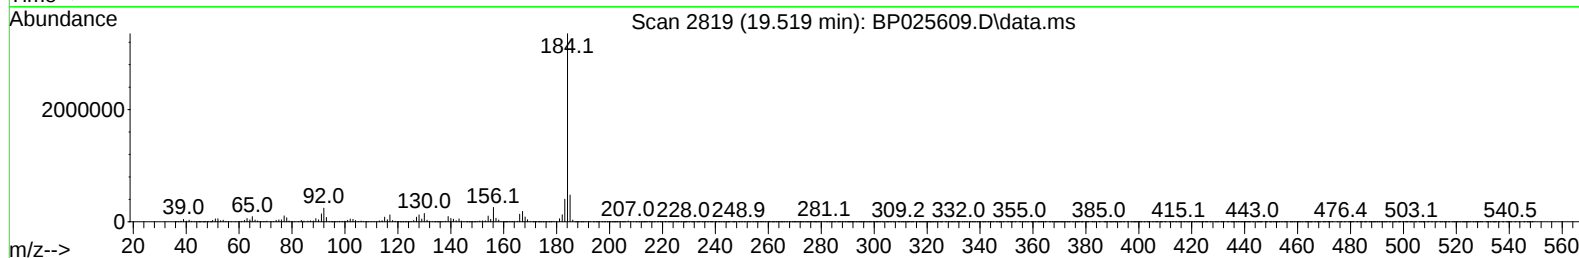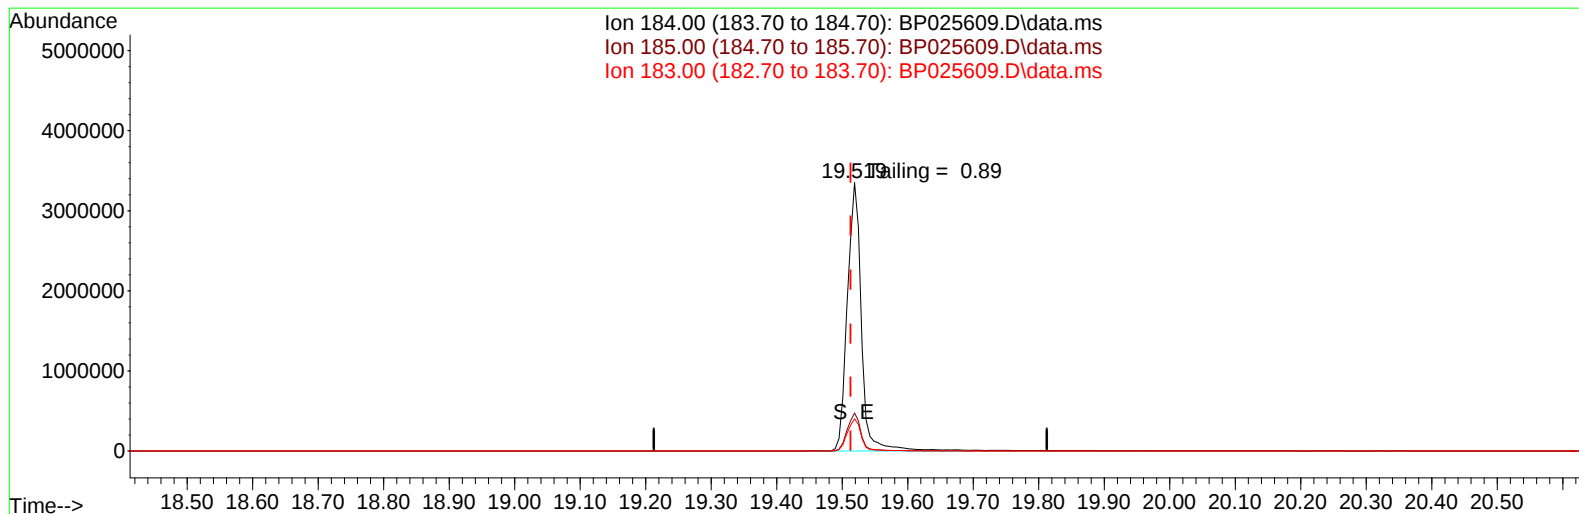

TIC: BP025609.D\data.ms

(77) Benzidine

19.519min (+ 0.006) 9970.21 ng




response 4932784

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.20
183.00	11.80	12.02
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082825\  
Data File : BP025609.D  
Acq On    : 28 Aug 2025  13:06  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 28 15:31:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Qlast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

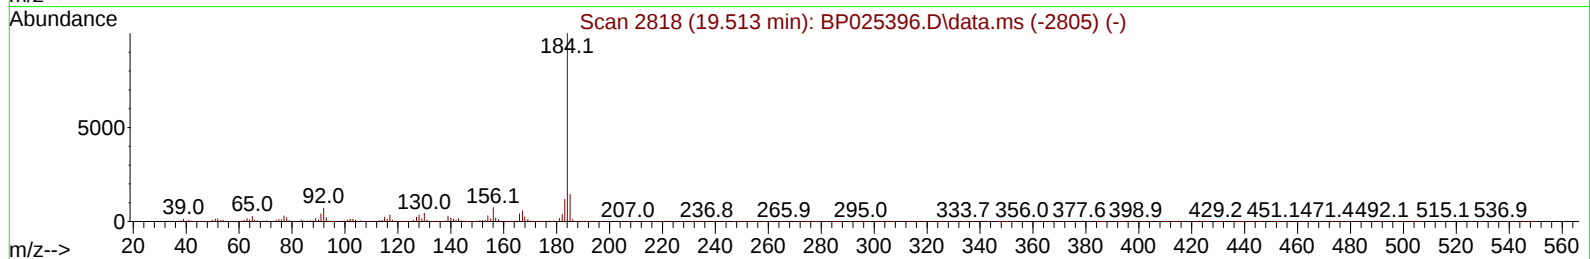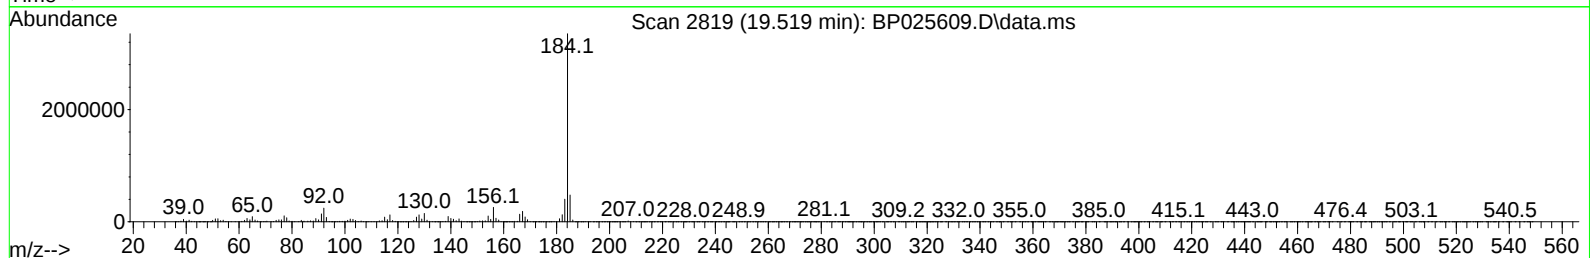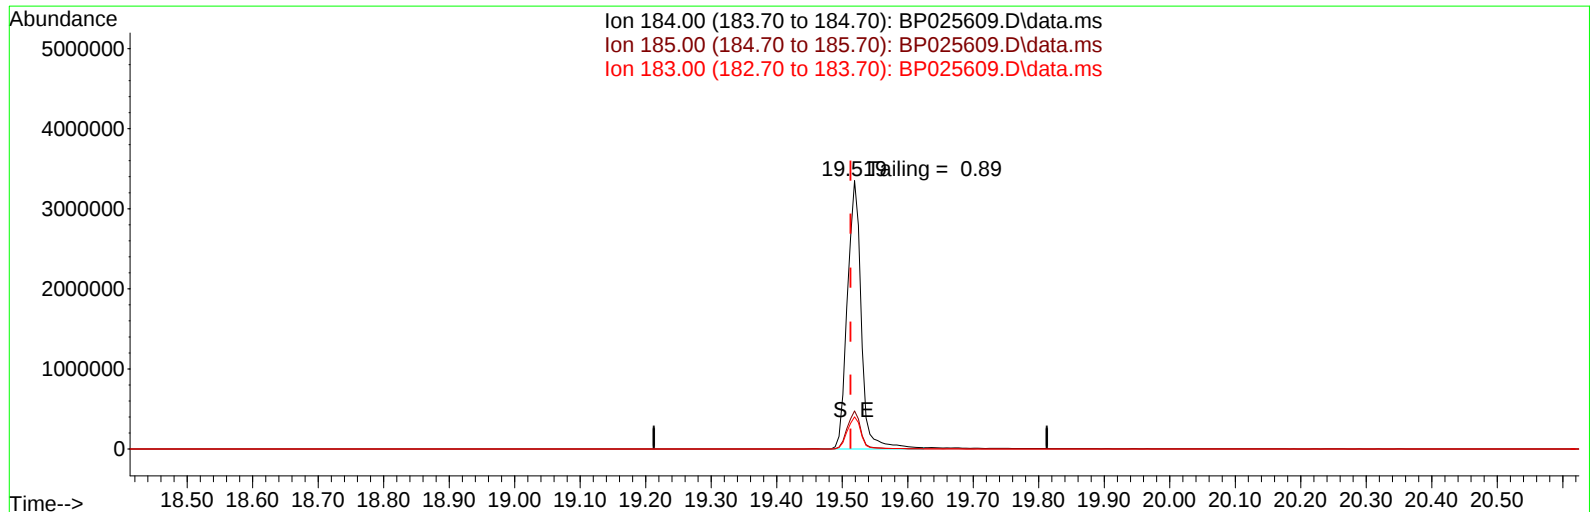

TIC: BP025609.D\data.ms

(77) Benzidine

19.519min (+ 0.006) 9970.21 ng

response 4932784

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.20
183.00	11.80	12.02
0.00	0.00	0.00