


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP083019\
 Data File : BP000004.D
 Acq On : 30 Aug 2019 14:08
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP083019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 30 17:47:17 2019

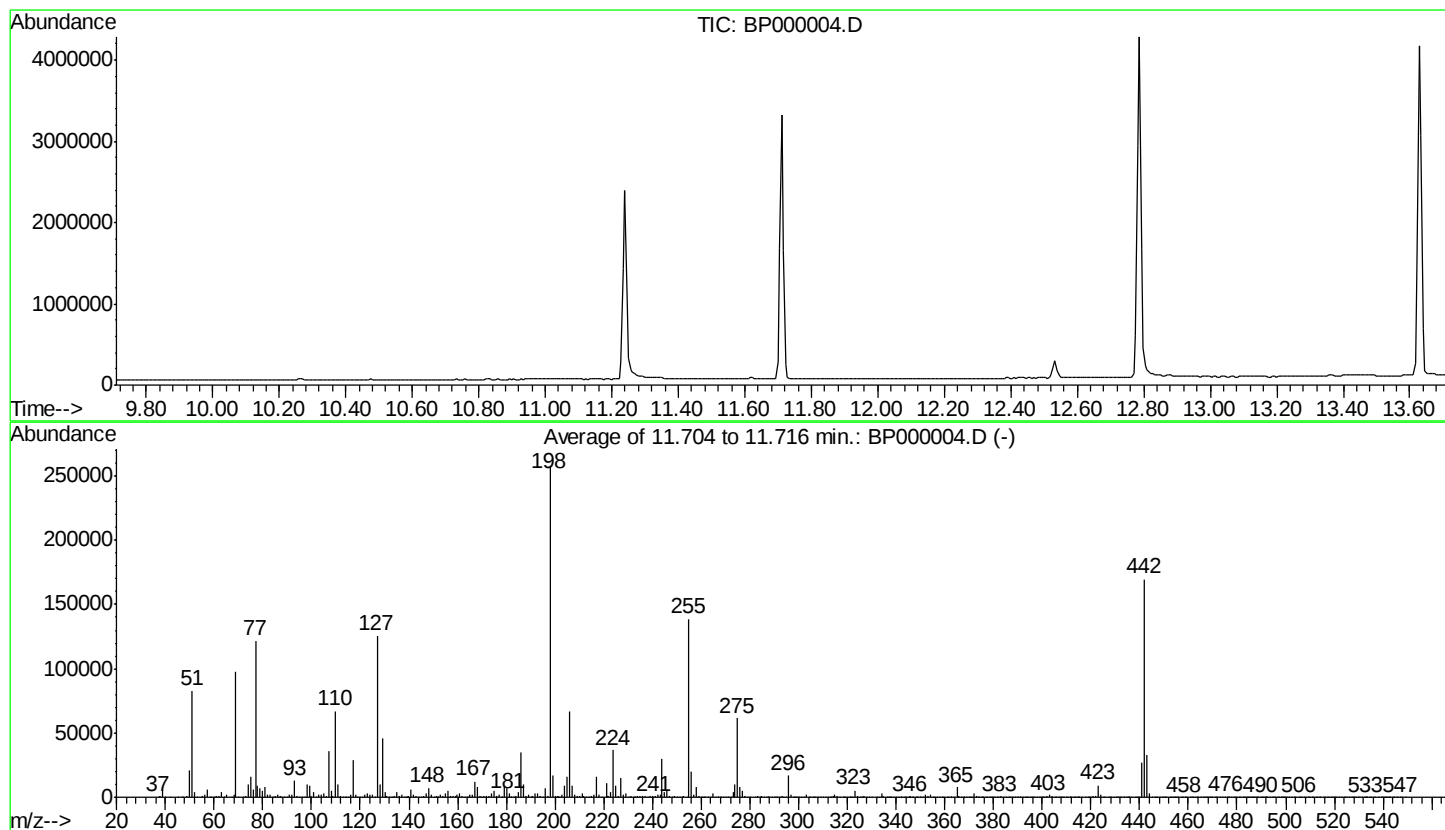

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1628

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.1	82866	PASS
68	69	0.00	2	1.8	1720	PASS
69	198	0.00	100	37.8	97470	PASS
70	69	0.00	2	0.5	509	PASS
127	198	10	80	48.7	125708	PASS
197	198	0.00	2	0.6	1519	PASS
198	198	100	100	100.0	258018	PASS
199	198	5	9	6.8	17425	PASS
275	198	10	60	23.9	61632	PASS
365	198	1	100	2.9	7533	PASS
441	198	0.01	100	10.5	27178	PASS
442	198	50	100	65.7	169586	PASS
443	442	15	24	19.6	33319	PASS