


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP083019\
 Data File : BP000013.D
 Acq On : 30 Aug 2019 19:09
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP083019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 30 17:47:17 2019

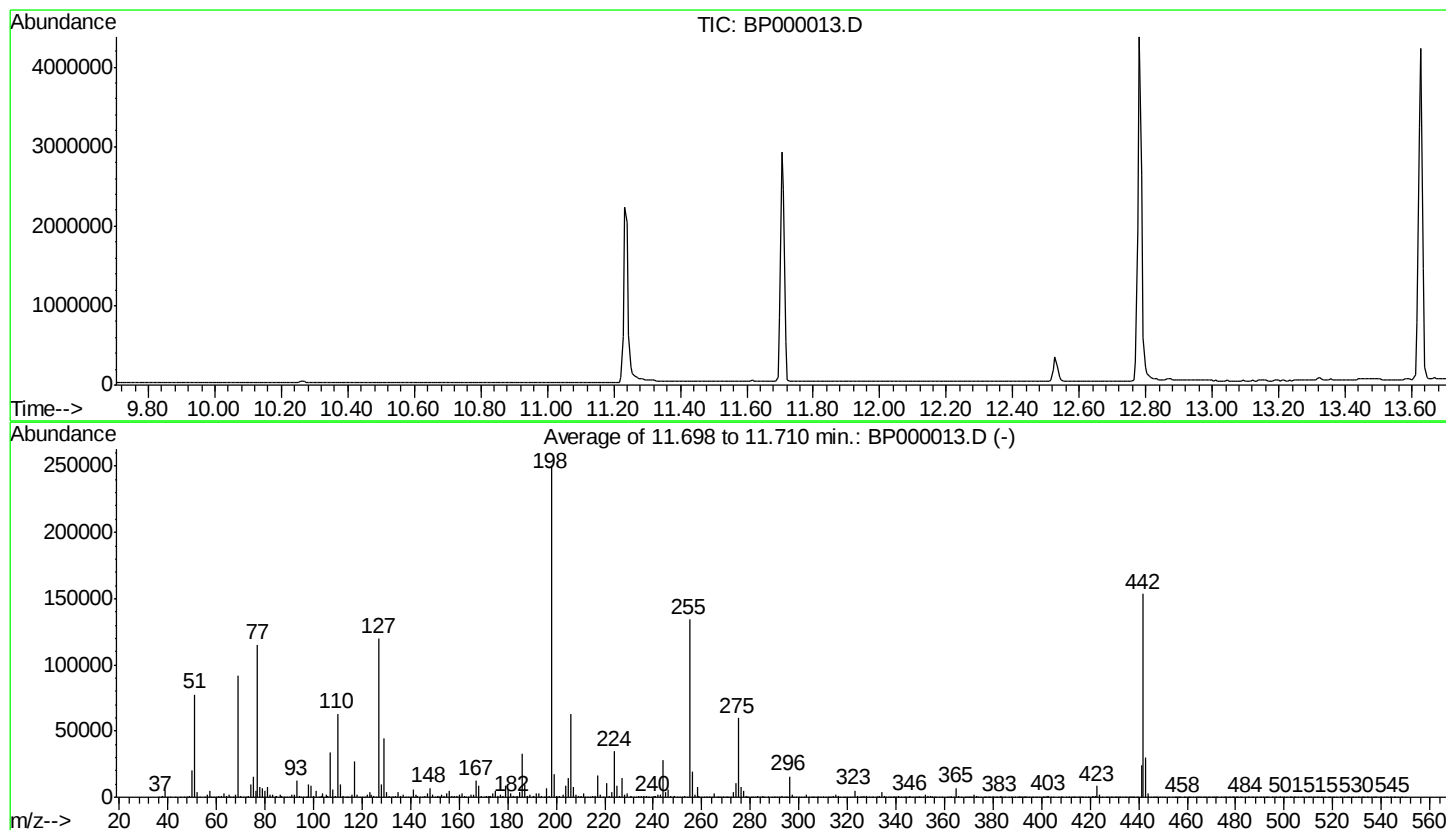

AutoFind: Scans 1634, 1635, 1636; Background Corrected with Scan 1628

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.1	77816	PASS
68	69	0.00	2	1.8	1623	PASS
69	198	0.00	100	36.6	91696	PASS
70	69	0.00	2	0.6	583	PASS
127	198	10	80	47.8	119696	PASS
197	198	0.00	2	0.2	611	PASS
198	198	100	100	100.0	250482	PASS
199	198	5	9	6.9	17205	PASS
275	198	10	60	23.8	59562	PASS
365	198	1	100	2.8	7048	PASS
441	198	0.01	100	9.6	24040	PASS
442	198	50	100	61.3	153596	PASS
443	442	15	24	19.8	30434	PASS