


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP083119\
 Data File : BP000028.D
 Acq On : 31 Aug 2019 07:09
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP083019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 30 17:47:17 2019

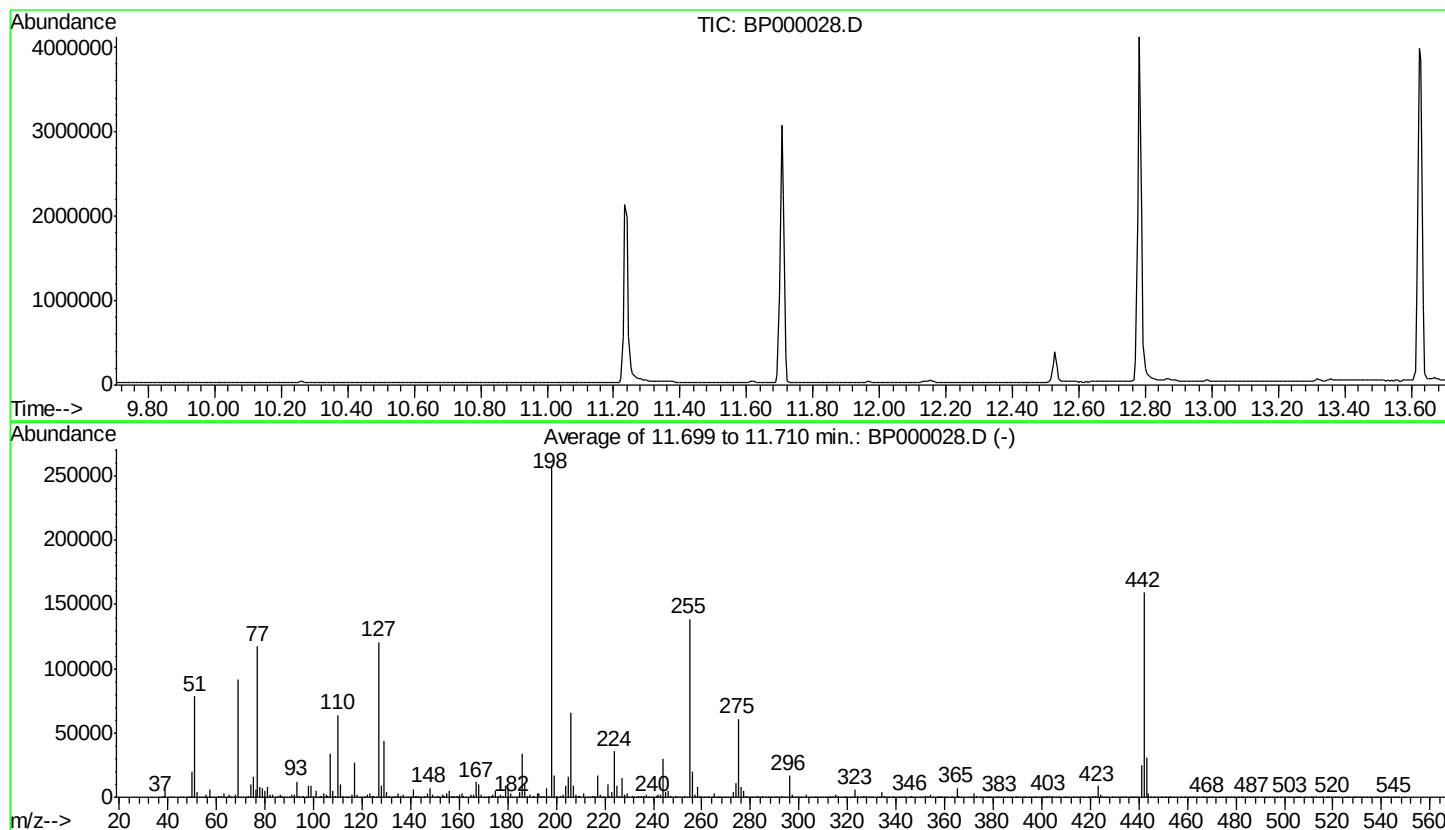

AutoFind: Scans 1634, 1635, 1636; Background Corrected with Scan 1628

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.3	78328	PASS
68	69	0.00	2	1.8	1625	PASS
69	198	0.00	100	35.4	91344	PASS
70	69	0.00	2	0.6	509	PASS
127	198	10	80	46.8	120834	PASS
197	198	0.00	2	0.6	1502	PASS
198	198	100	100	100.0	258120	PASS
199	198	5	9	6.8	17442	PASS
275	198	10	60	23.7	61253	PASS
365	198	1	100	2.7	7051	PASS
441	198	0.01	100	9.6	24699	PASS
442	198	50	100	61.7	159335	PASS
443	442	15	24	19.5	31103	PASS