

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP083123\
 Data File : BP016890.D
 Acq On : 31 Aug 2023 10:46
 Operator : MA/JU
 Sample : PB155141BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK141

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016890.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.376	11	15	28	rVB	138186	210463	2.13%	0.209%
2	3.811	84	89	116	rBV	1443071	2448687	24.83%	2.436%
3	4.123	138	142	153	rVB	63342	100213	1.02%	0.100%
4	7.164	651	659	672	rBV	1802878	2904346	29.45%	2.889%
5	7.358	685	692	701	rVB	1505139	2280532	23.12%	2.268%
6	7.534	715	722	737	rBV	1733230	2769965	28.09%	2.755%
7	8.017	794	804	816	rBV	1288135	2037937	20.66%	2.027%
8	8.722	915	924	941	rBV	2248118	3605146	36.55%	3.586%
9	9.216	1000	1008	1019	rBV	1767982	2871209	29.11%	2.856%
10	9.928	1117	1129	1142	rBV	1390635	2318862	23.51%	2.307%
11	10.452	1210	1218	1241	rBV	2135146	3636281	36.87%	3.617%
12	10.846	1278	1285	1299	rBV	1973472	3231757	32.77%	3.215%
13	11.005	1304	1312	1340	rBV	2241227	3816490	38.70%	3.796%
14	12.428	1548	1554	1563	rBV	35527	63631	0.65%	0.063%
15	13.516	1732	1739	1744	rBV3	15290	24885	0.25%	0.025%
16	13.634	1756	1759	1765	rVB7	6341	9915	0.10%	0.010%
17	14.081	1828	1835	1848	rBV	3898646	5429565	55.05%	5.401%
18	14.369	1878	1884	1899	rBV	4447104	6601775	66.94%	6.567%
19	14.675	1927	1936	1953	rBV	3027900	4437769	45.00%	4.414%
20	14.875	1964	1970	1988	rBV	1221880	2317763	23.50%	2.305%
21	15.669	2098	2105	2116	rBV	5885671	8274339	83.90%	8.230%
22	15.787	2119	2125	2140	rVV	1321014	1893335	19.20%	1.883%
23	15.904	2141	2145	2154	rVB	27752	48647	0.49%	0.048%
24	17.110	2345	2350	2354	rVB7	9459	15158	0.15%	0.015%
25	17.222	2366	2369	2375	rBV4	8544	14730	0.15%	0.015%
26	17.440	2400	2406	2416	rBV	3660506	5214021	52.87%	5.186%
27	17.540	2417	2423	2444	rVB	6426685	9060042	91.87%	9.012%
28	19.351	2727	2731	2735	rVB	65083	85936	0.87%	0.085%
29	19.416	2739	2742	2750	rVB	56845	81382	0.83%	0.081%
30	19.775	2797	2803	2816	rBV	7731137	9862261	100.00%	9.810%
31	21.539	3098	3103	3112	rBV	3270077	4307337	43.67%	4.284%
32	23.939	3503	3511	3524	rVB2	3260626	6903277	70.00%	6.867%
33	24.110	3533	3540	3553	rVB	1683207	3657174	37.08%	3.638%




Sum of corrected areas: 100534830

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP083123\
Data File : BP016890.D
Acq On : 31 Aug 2023 10:46
Operator : MA/JU
Sample : PB155141BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK141

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

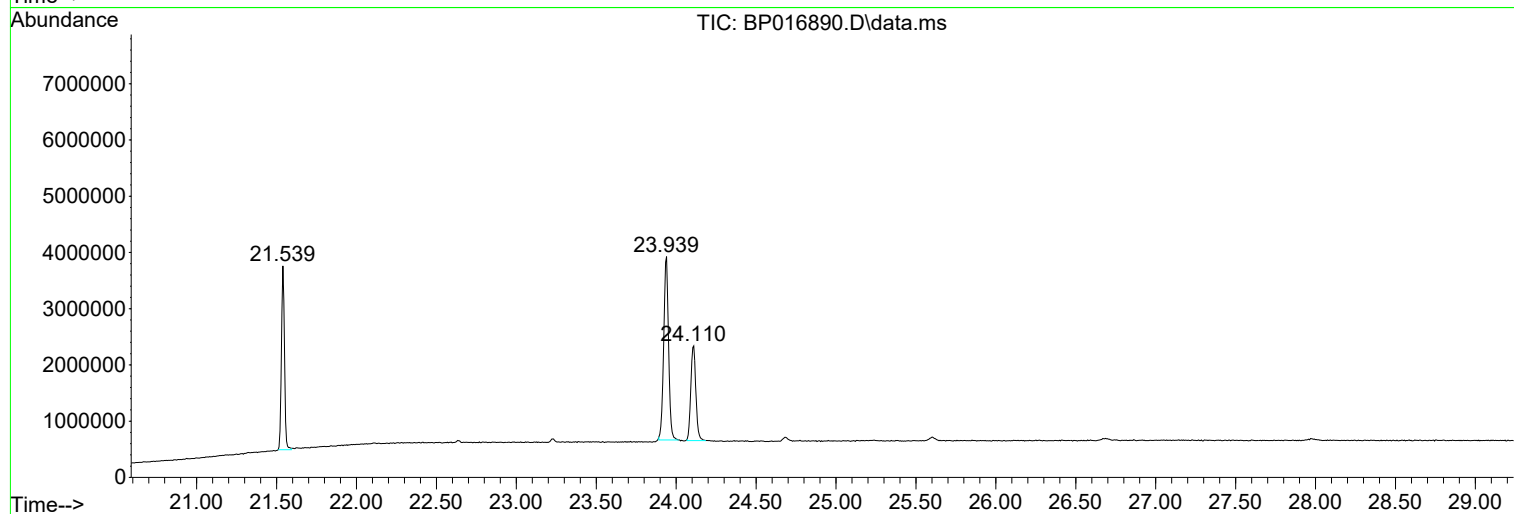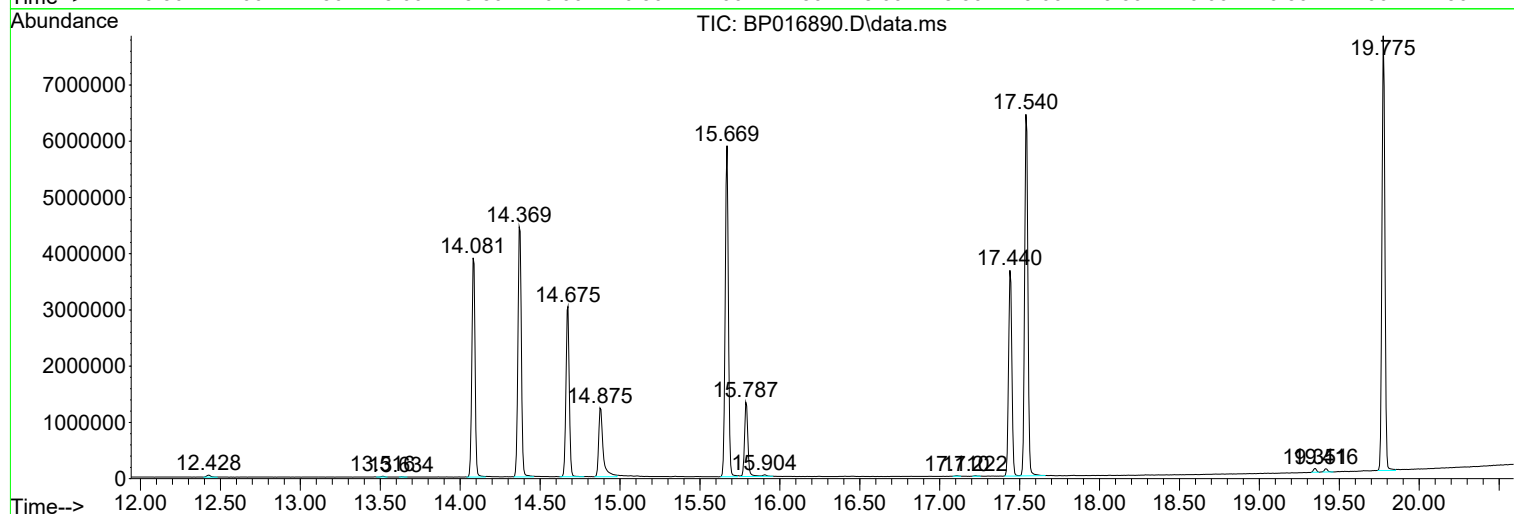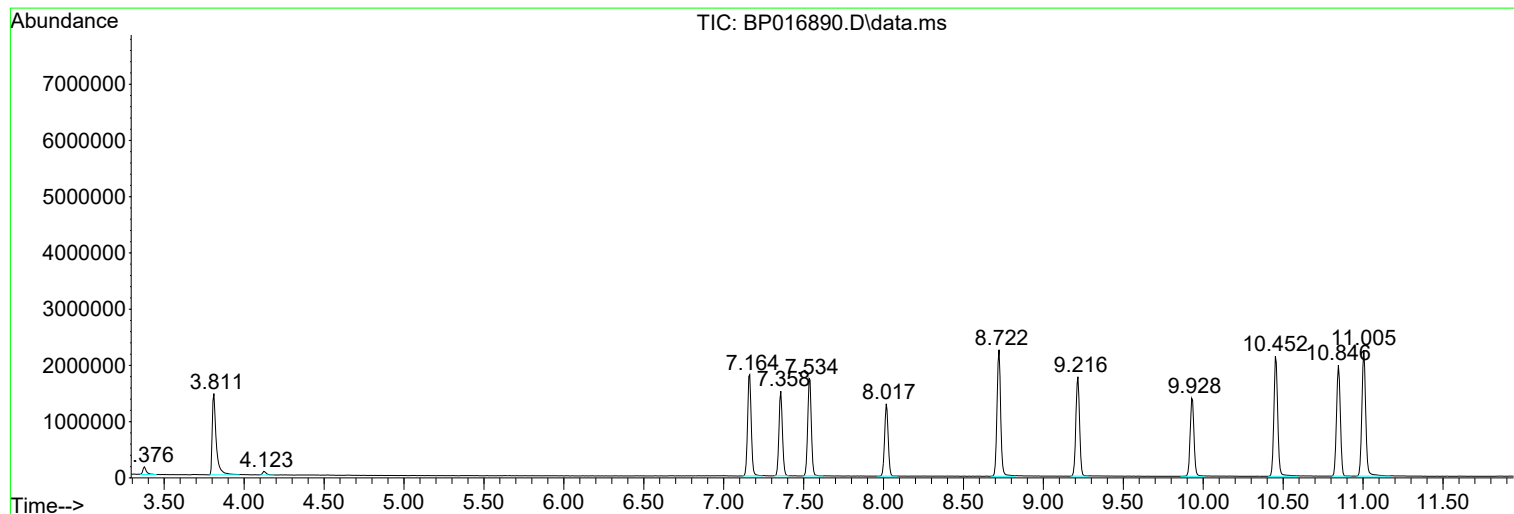

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP083123\
Data File : BP016890.D
Acq On : 31 Aug 2023 10:46
Operator : MA/JU
Sample : PB155141BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK141

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP083123\
Data File : BP016890.D
Acq On : 31 Aug 2023 10:46
Operator : MA/JU
Sample : PB155141BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK141

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------