

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
 Data File : BP016908.D
 Acq On : 01 Sep 2023 15:22
 Operator : MA/JU
 Sample : 04134-07
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCHK0

Quant Time: Sep 01 22:38:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 30 02:25:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.022	152	329705	20.000	ng/u1	0.00
20) Naphthalene-d8	10.846	136	1423835	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.675	164	887835	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.445	188	1935873	20.000	ng/u1	0.00
79) Chrysene-d12	21.545	240	1586992	20.000	ng/u1	0.00
88) Perylene-d12	24.110	264	1534943	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	51623	6.471	ng/uL	0.00
4) Pyridine-d5	3.811	84	305907	12.548	ng/u1	0.00
7) Phenol-d5	7.169	99	255194	8.704	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.358	67	646643	34.607	ng/u1	0.00
11) 2-Chlorophenol-d4	7.540	132	619376	28.099	ng/u1	0.00
15) 4-Methylphenol-d8	8.728	113	446263	18.646	ng/u1	0.00
21) Nitrobenzene-d5	9.216	128	406025	37.715	ng/u1	0.00
24) 2-Nitrophenol-d4	9.934	143	430350	37.924	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.457	165	714904	33.793	ng/u1	0.00
31) 4-Chloroaniline-d4	11.004	131	876166	27.006	ng/u1	0.00
46) Dimethylphthalate-d6	14.087	166	2665130	39.805	ng/u1	0.00
49) Acenaphthylene-d8	14.375	160	2850386	37.659	ng/u1	0.00
54) 4-Nitrophenol-d4	14.898	143	118165	8.539	ng/u1	0.01
60) Fluorene-d10	15.669	176	2228950	39.532	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.798	200	449614	38.999	ng/u1	0.00
73) Anthracene-d10	17.545	188	3762608	43.849	ng/u1	0.00
81) Pyrene-d10	19.780	212	4260802	48.885	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.945	264	3395012	44.156	ng/u1	0.00
Target Compounds						
					Qvalue	
58) 2,3,4,6-Tetrachlorophenol	15.292	232	22241	1.429	ng/u1#	96
71) Pentachlorophenol	17.069	266	98113	6.360	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016908.D
Acq On : 01 Sep 2023 15:22
Operator : MA/JU
Sample : 04134-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHK0

Quant Time: Sep 01 22:38:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 30 02:25:00 2023
Response via : Initial Calibration




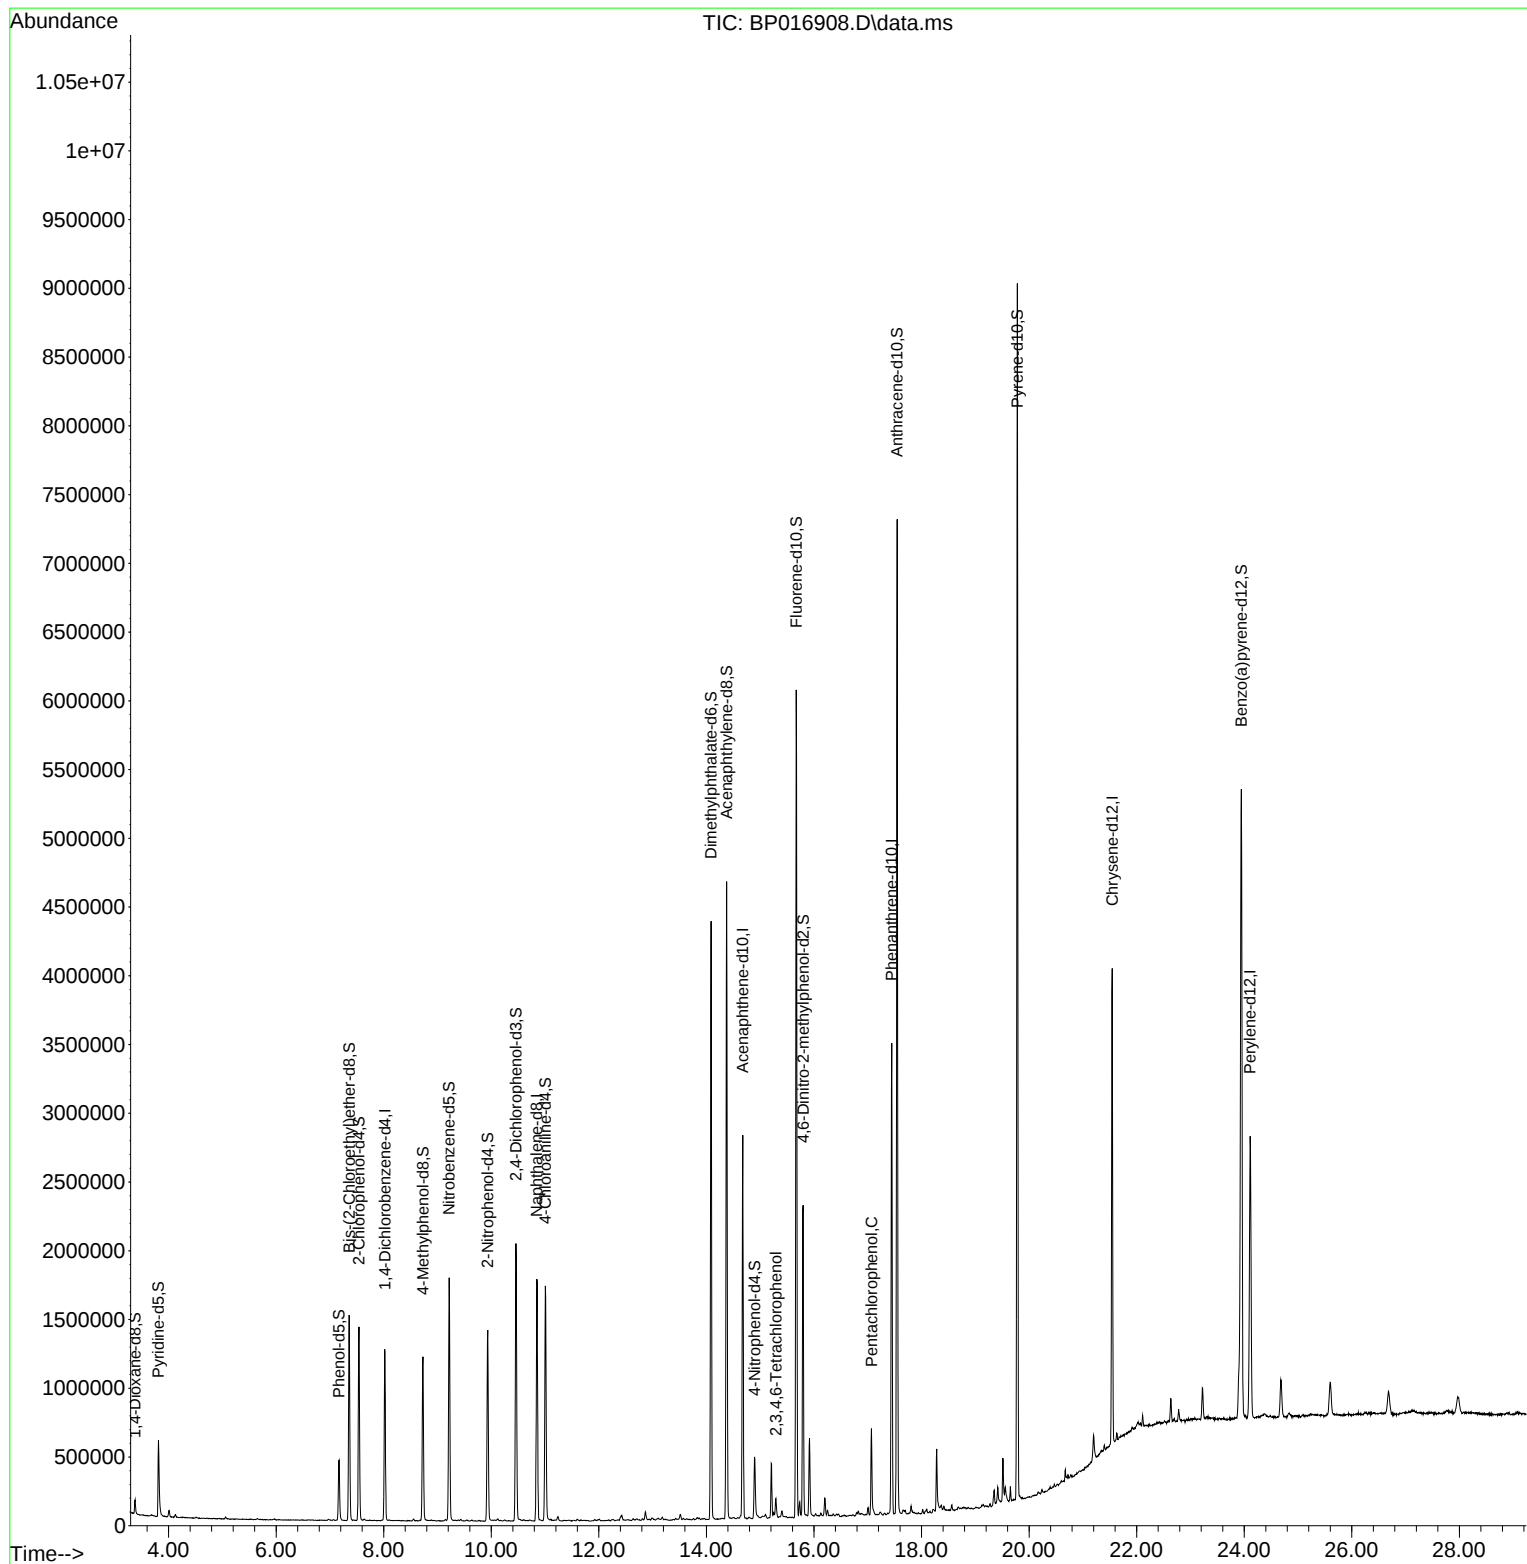


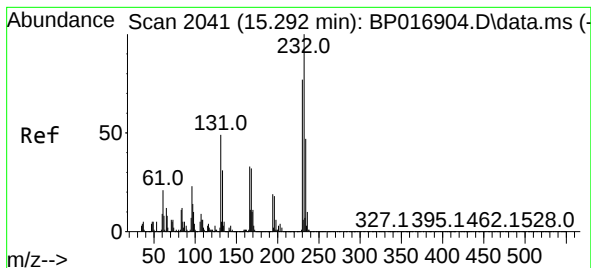

#58
2,3,4,6-Tetrachlorophenol
Concen: 1.429 ng/ul
RT: 15.292 min Scan# 2041
Delta R.T. 0.000 min
Lab File: BP016908.D
Acq: 01 Sep 2023 15:22

Instrument :
BNA_P
ClientSampleId :
DCHK0

Tgt Ion:232	Resp:	22241
Ion Ratio	Lower	Upper
232	100	
131	48.2	38.1 57.1
130	3.1	1.9 2.9#
166	37.4	26.5 39.7

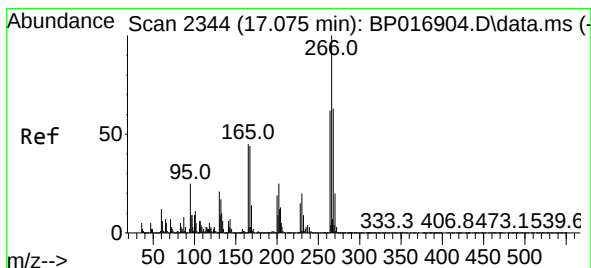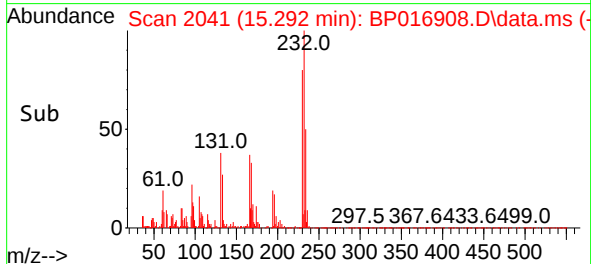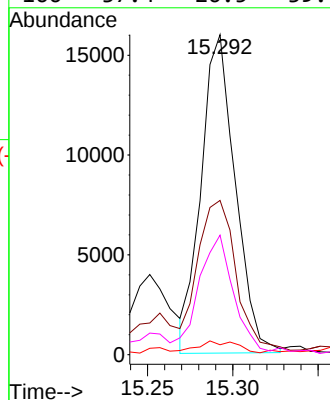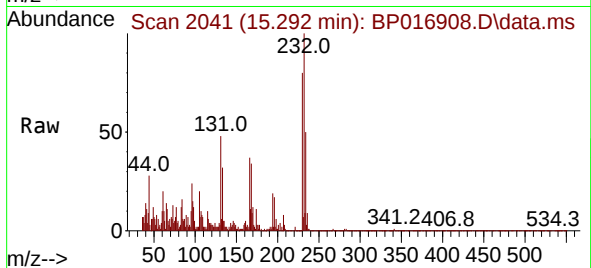

#71
Pentachlorophenol
Concen: 6.360 ng/ul
RT: 17.069 min Scan# 2343
Delta R.T. 0.000 min
Lab File: BP016908.D
Acq: 01 Sep 2023 15:22

Tgt Ion:266	Resp:	98113
Ion Ratio	Lower	Upper
266	100	
264	64.5	50.7 76.1
268	64.4	50.8 76.2

