

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
 Data File : BP016909.D
 Acq On : 01 Sep 2023 15:56
 Operator : MA/JU
 Sample : 04134-08
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCHK1

Quant Time: Sep 01 23:16:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 30 02:25:00 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.022	152	321668	20.000	ng/u1	0.00
20) Naphthalene-d8	10.846	136	1398965	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.675	164	904724	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.445	188	1973565	20.000	ng/u1	0.00
79) Chrysene-d12	21.545	240	1622998	20.000	ng/u1	0.00
88) Perylene-d12	24.116	264	1590252	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	39349	5.056	ng/uL	0.00
4) Pyridine-d5	3.811	84	204347	8.592	ng/u1	0.00
7) Phenol-d5	7.169	99	202806	7.090	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.358	67	575048	31.544	ng/u1	0.00
11) 2-Chlorophenol-d4	7.540	132	545676	25.374	ng/u1	0.00
15) 4-Methylphenol-d8	8.728	113	362207	15.512	ng/u1	0.00
21) Nitrobenzene-d5	9.216	128	359838	34.019	ng/u1	0.00
24) 2-Nitrophenol-d4	9.934	143	384612	34.496	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.457	165	642808	30.925	ng/u1	0.00
31) 4-Chloroaniline-d4	11.004	131	700074	21.962	ng/u1	0.00
46) Dimethylphthalate-d6	14.087	166	2323240	34.051	ng/u1	0.00
49) Acenaphthylene-d8	14.375	160	2555488	33.132	ng/u1	0.00
54) 4-Nitrophenol-d4	14.892	143	83325	5.909	ng/u1	0.00
60) Fluorene-d10	15.669	176	1992851	34.685	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.798	200	351606	29.916	ng/u1	0.00
73) Anthracene-d10	17.545	188	3250370	37.156	ng/u1	0.00
81) Pyrene-d10	19.780	212	3671832	41.193	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.945	264	2927347	36.749	ng/u1	0.00
Target Compounds						
71) Pentachlorophenol	17.069	266	36240	2.304	ng/u1	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016909.D
Acq On : 01 Sep 2023 15:56
Operator : MA/JU
Sample : 04134-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHK1

Quant Time: Sep 01 23:16:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 30 02:25:00 2023
Response via : Initial Calibration

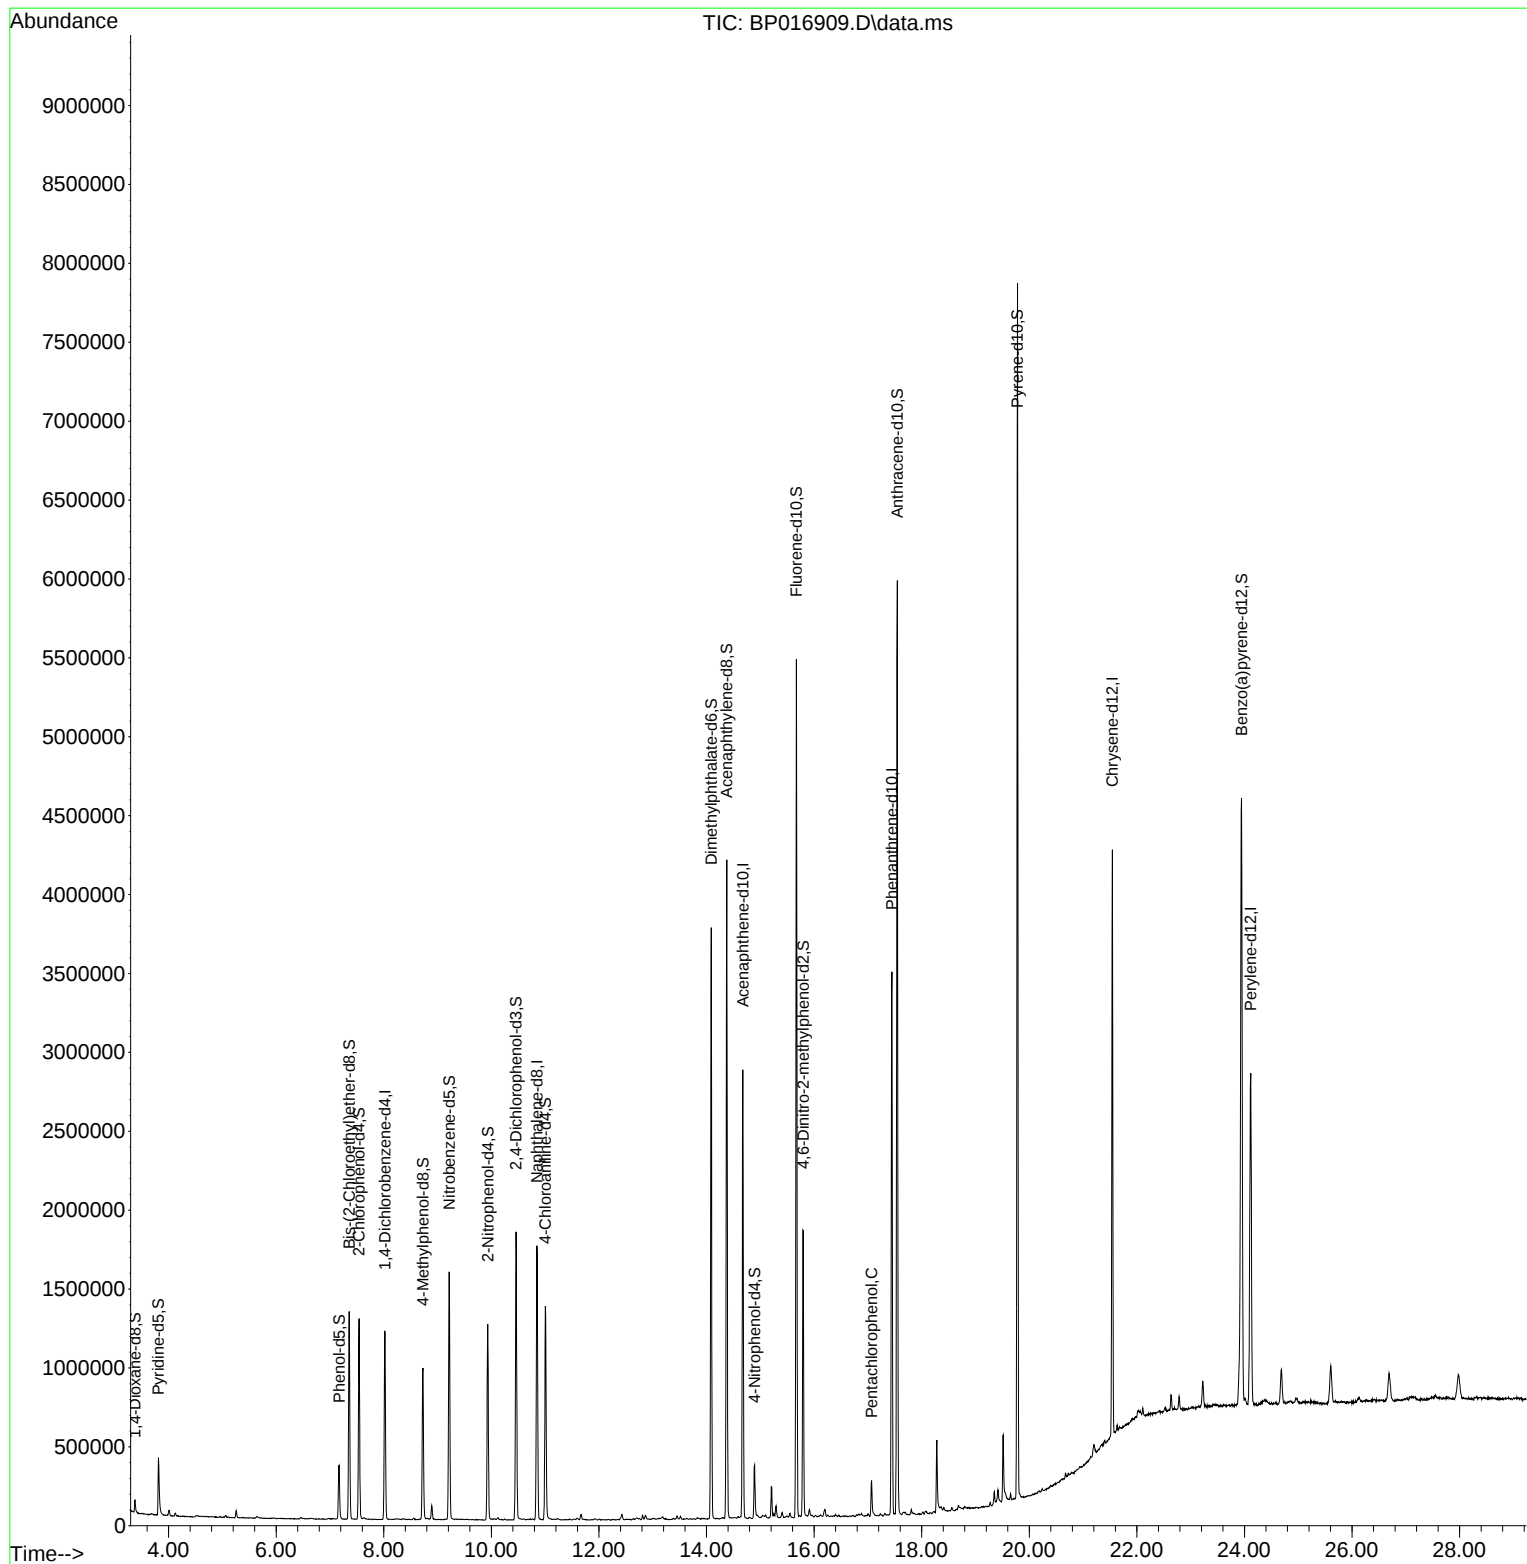

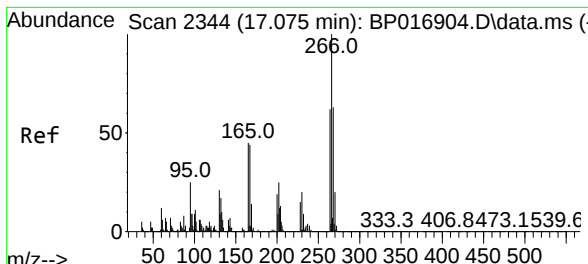

#71
 Pentachlorophenol
 Concen: 2.304 ng/ul
 RT: 17.069 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BP016909.D
 Acq: 01 Sep 2023 15:56

Instrument :
 BNA_P
 ClientSampleId :
 DCHK1

Tgt Ion:	266	Resp:	36240
Ion Ratio	Lower	Upper	
266	100		
264	61.9	50.7	76.1
268	61.3	50.8	76.2

