

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
 Data File : BP016913.D
 Acq On : 01 Sep 2023 18:12
 Operator : MA/JU
 Sample : 04113-15
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYJ1

Quant Time: Sep 01 23:32:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 30 02:25:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.022	152	340730	20.000	ng/u1	0.00
20) Naphthalene-d8	10.851	136	1464344	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.675	164	893667	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.445	188	1920541	20.000	ng/u1	0.00
79) Chrysene-d12	21.545	240	1678221	20.000	ng/u1	0.00
88) Perylene-d12	24.121	264	1561084	20.000	ng/u1	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	24284	2.946	ng/uL	0.00
4) Pyridine-d5	3.822	84	23107	0.917	ng/u1	0.01
7) Phenol-d5	7.169	99	471470	15.561	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.357	67	314802	16.302	ng/u1	0.00
11) 2-Chlorophenol-d4	7.540	132	371291	16.299	ng/u1	0.00
15) 4-Methylphenol-d8	8.728	113	260042	10.514	ng/u1	0.00
21) Nitrobenzene-d5	9.216	128	190265	17.185	ng/u1	0.00
24) 2-Nitrophenol-d4	9.934	143	210353	18.024	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.457	165	360864	16.586	ng/u1	0.00
31) 4-Chloroaniline-d4	11.010	131	129835	3.891	ng/u1	0.00
46) Dimethylphthalate-d6	14.086	166	1185962	17.597	ng/u1	0.00
49) Acenaphthylene-d8	14.375	160	1371023	17.995	ng/u1	0.00
54) 4-Nitrophenol-d4	14.886	143	162797	11.687	ng/u1	0.00
60) Fluorene-d10	15.669	176	1057541	18.634	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.798	200	98338	8.598	ng/u1	0.00
73) Anthracene-d10	17.545	188	1553155	18.245	ng/u1	0.00
81) Pyrene-d10	19.780	212	1935160	20.995	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.945	264	1468656	18.782	ng/u1	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.869	105	63142	1.646	ng/u1	97
36) 2-Methylnaphthalene	12.498	142	66910	1.278	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016913.D
Acq On : 01 Sep 2023 18:12
Operator : MA/JU
Sample : 04113-15
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYJ1

Quant Time: Sep 01 23:32:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 30 02:25:00 2023
Response via : Initial Calibration




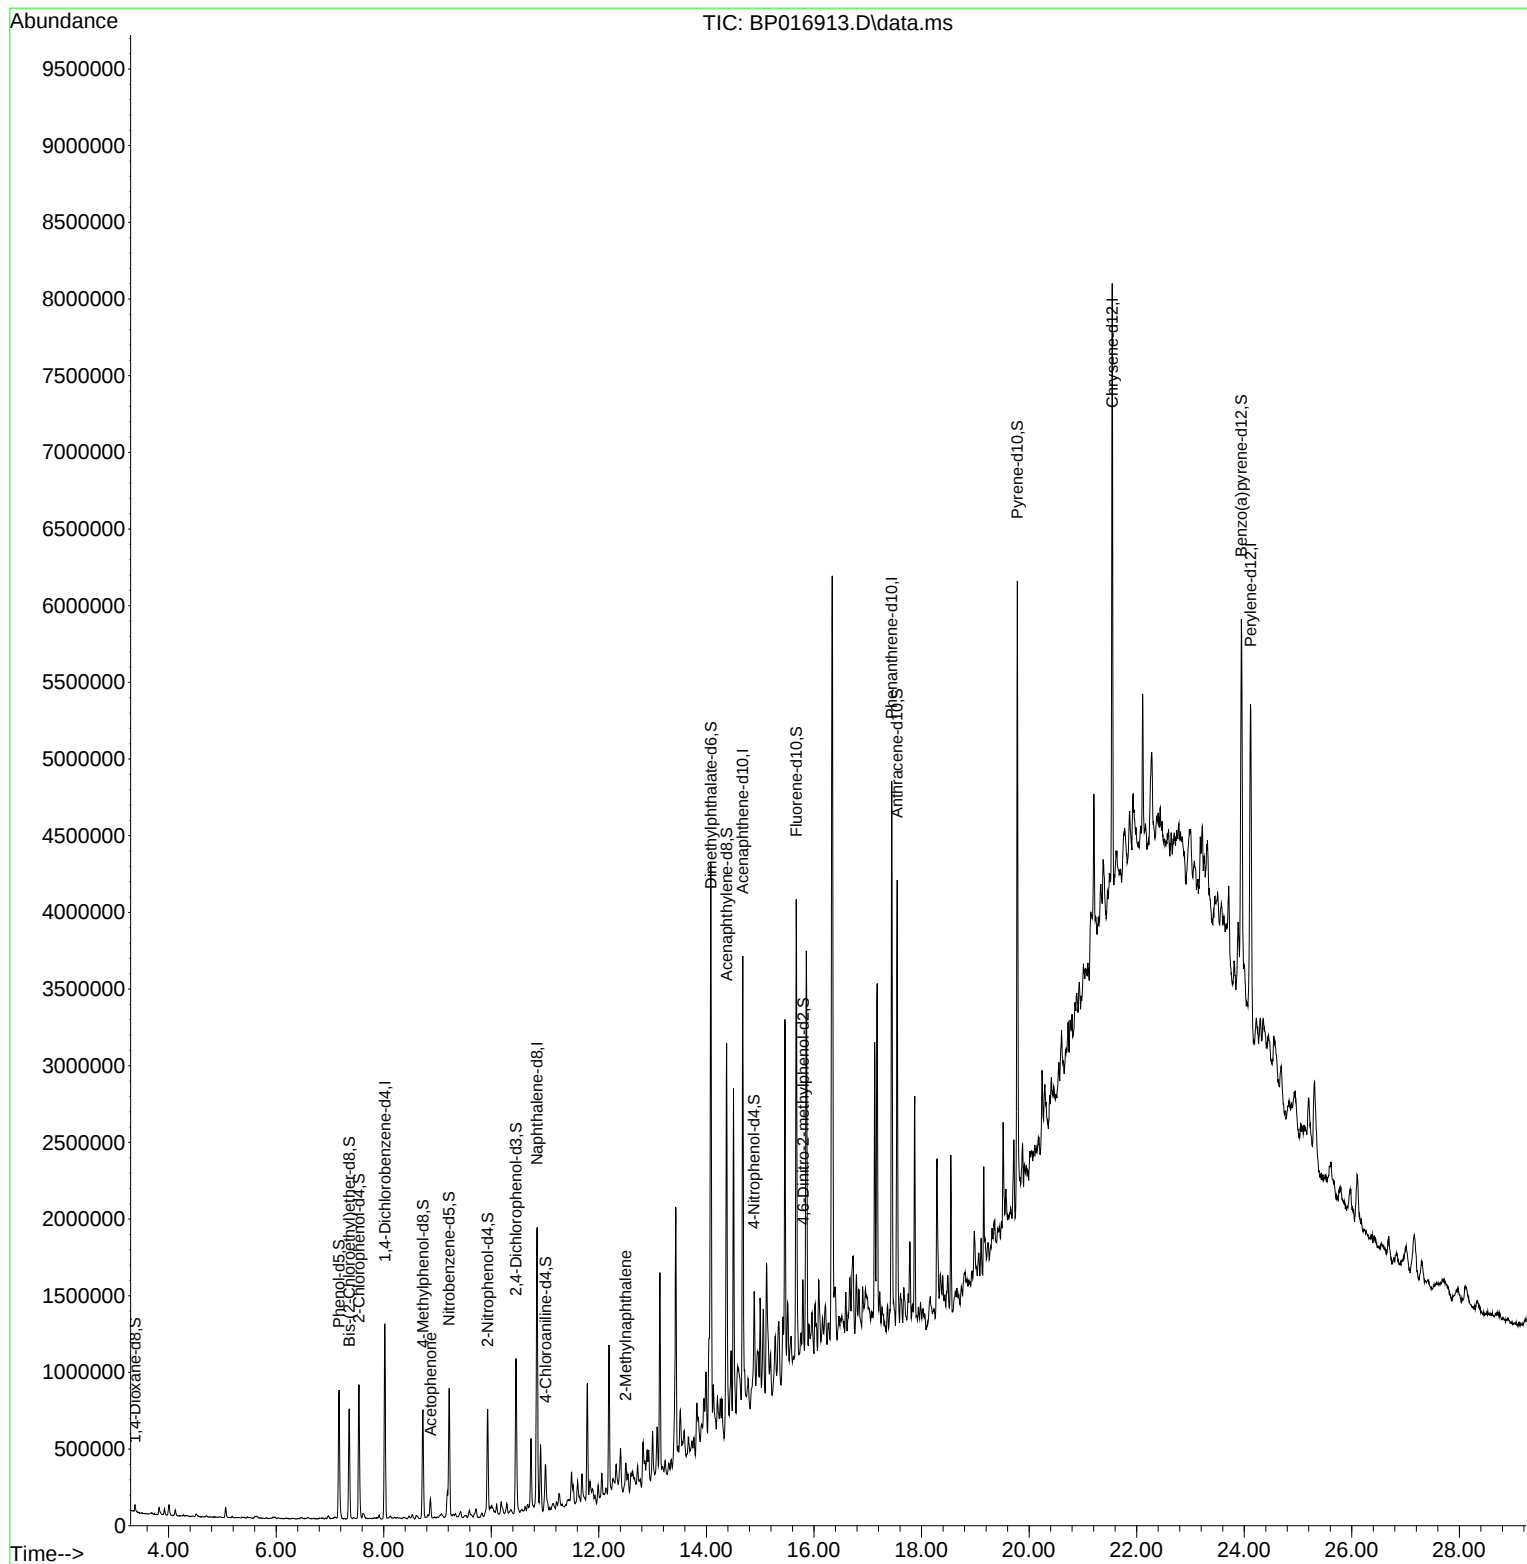


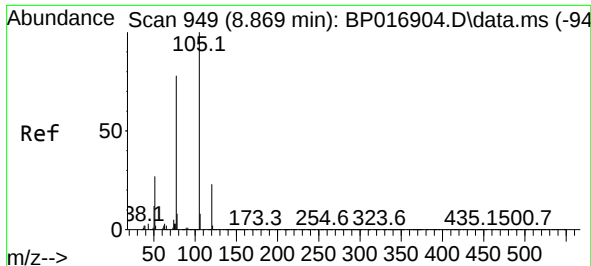

#16
Acetophenone
Concen: 1.646 ng/ul
RT: 8.869 min Scan# 949
Delta R.T. -0.006 min
Lab File: BP016913.D
Acq: 01 Sep 2023 18:12

Instrument :
BNA_P
ClientSampleId :
EZYJ1

Tgt Ion:105 Resp: 63142
Ion Ratio Lower Upper
105 100
77 82.4 64.2 96.4
51 30.5 22.2 33.4

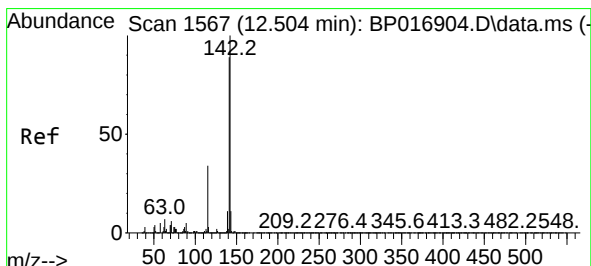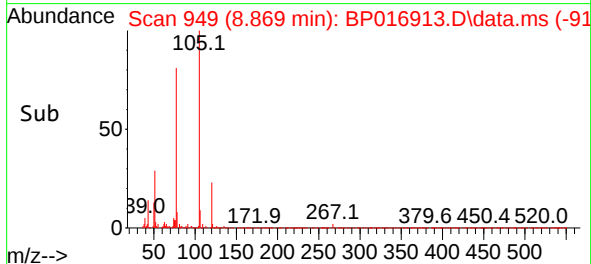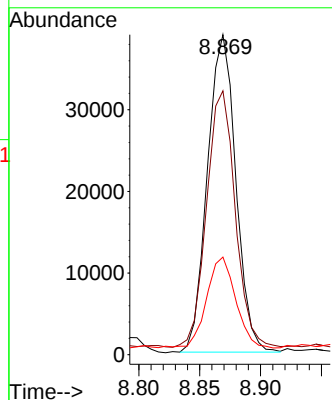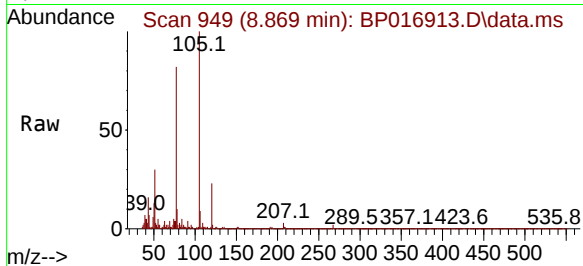

#36
2-Methylnaphthalene
Concen: 1.278 ng/ul
RT: 12.498 min Scan# 1566
Delta R.T. -0.006 min
Lab File: BP016913.D
Acq: 01 Sep 2023 18:12

Tgt Ion:142 Resp: 66910
Ion Ratio Lower Upper
142 100
141 91.3 71.4 107.0

