

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
 Data File : BP016914.D
 Acq On : 01 Sep 2023 18:46
 Operator : MA/JU
 Sample : 04113-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYH5

Quant Time: Sep 01 23:39:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 30 02:25:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	332633	20.000	ng/u1	0.00
20) Naphthalene-d8	10.851	136	1500972	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.675	164	985392	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.445	188	2130720	20.000	ng/u1	0.00
79) Chrysene-d12	21.539	240	1609072	20.000	ng/u1	0.00
88) Perylene-d12	24.110	264	1482449	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	23549	2.926	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	7.169	99	434180	14.679	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.357	67	285899	15.166	ng/u1	0.00
11) 2-Chlorophenol-d4	7.540	132	339717	15.276	ng/u1	0.00
15) 4-Methylphenol-d8	8.728	113	245613	10.172	ng/u1	0.00
21) Nitrobenzene-d5	9.216	128	170780	15.048	ng/u1	0.00
24) 2-Nitrophenol-d4	9.934	143	193654	16.188	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.457	165	334481	14.998	ng/u1	0.00
31) 4-Chloroaniline-d4	11.010	131	229349	6.706	ng/u1	0.00
46) Dimethylphthalate-d6	14.087	166	1184169	15.935	ng/u1	0.00
49) Acenaphthylene-d8	14.375	160	1320879	15.723	ng/u1	0.00
54) 4-Nitrophenol-d4	14.886	143	135824	8.843	ng/u1	0.00
60) Fluorene-d10	15.669	176	1020665	16.310	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.792	200	93773	7.390	ng/u1	0.00
73) Anthracene-d10	17.545	188	1510234	15.991	ng/u1	0.00
81) Pyrene-d10	19.780	212	1789076	20.245	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.939	264	1261073	16.982	ng/u1	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.869	105	87970	2.350	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016914.D
Acq On : 01 Sep 2023 18:46
Operator : MA/JU
Sample : 04113-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYH5

Quant Time: Sep 01 23:39:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 30 02:25:00 2023
Response via : Initial Calibration

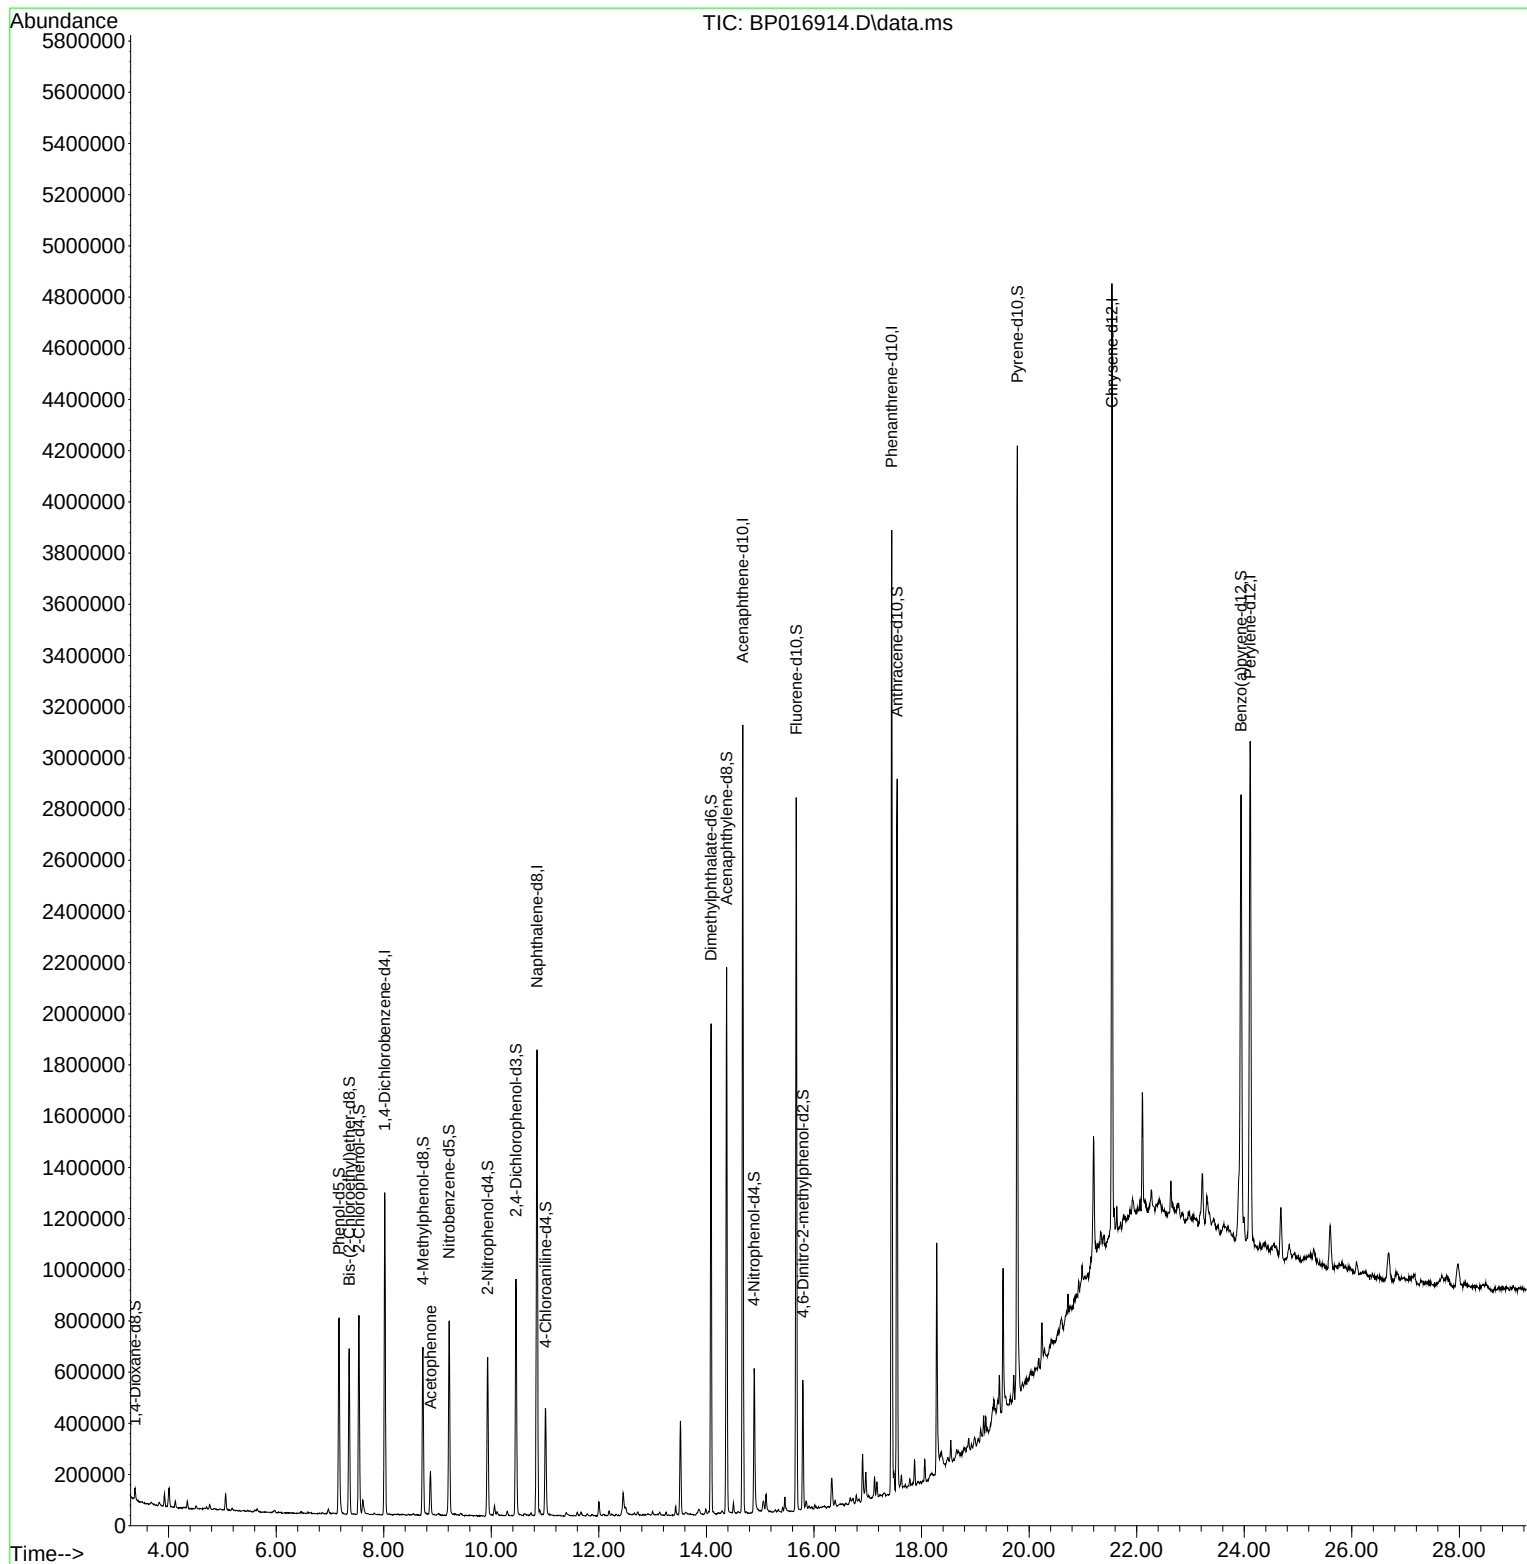

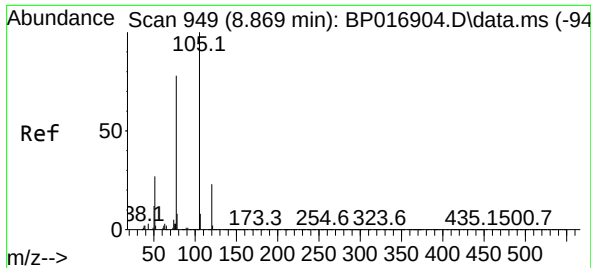

#16
 Acetophenone
 Concen: 2.350 ng/ul
 RT: 8.869 min Scan# 94
 Delta R.T. -0.006 min
 Lab File: BP016914.D
 Acq: 01 Sep 2023 18:46

Instrument :
 BNA_P
 ClientSampleId :
 EZYH5

Tgt Ion:105 Resp: 87970
 Ion Ratio Lower Upper
 105 100
 77 80.1 64.2 96.4
 51 29.3 22.2 33.4

