

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
 Data File : BP016917.D
 Acq On : 01 Sep 2023 20:28
 Operator : MA/JU
 Sample : 04123-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH942

Quant Time: Sep 01 23:43:38 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 30 02:25:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	320416	20.000	ng/u1	0.00
20) Naphthalene-d8	10.846	136	1414389	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.675	164	907893	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.445	188	1997962	20.000	ng/u1	0.00
79) Chrysene-d12	21.545	240	1726536	20.000	ng/u1	0.00
88) Perylene-d12	24.115	264	1655475	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	45915	5.922	ng/uL	0.00
4) Pyridine-d5	3.811	84	221065	9.331	ng/u1	0.00
7) Phenol-d5	7.163	99	221256	7.766	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.358	67	624352	34.383	ng/u1	0.00
11) 2-Chlorophenol-d4	7.540	132	581309	27.136	ng/u1	0.00
15) 4-Methylphenol-d8	8.728	113	416143	17.892	ng/u1	0.00
21) Nitrobenzene-d5	9.216	128	385867	36.082	ng/u1	0.00
24) 2-Nitrophenol-d4	9.934	143	420965	37.345	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.457	165	727065	34.597	ng/u1	0.00
31) 4-Chloroaniline-d4	11.004	131	804936	24.977	ng/u1	0.00
46) Dimethylphthalate-d6	14.087	166	2700314	39.439	ng/u1	0.00
49) Acenaphthylene-d8	14.375	160	2960899	38.254	ng/u1	0.00
54) 4-Nitrophenol-d4	14.887	143	107327	7.584	ng/u1	0.00
60) Fluorene-d10	15.669	176	2301749	39.921	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.792	200	439660	36.951	ng/u1	0.00
73) Anthracene-d10	17.545	188	3829262	43.239	ng/u1	0.00
81) Pyrene-d10	19.780	212	4416769	46.578	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.945	264	3617871	43.628	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.411	88	23239	2.753	ng/uL	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016917.D
Acq On : 01 Sep 2023 20:28
Operator : MA/JU
Sample : 04123-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH942

Quant Time: Sep 01 23:43:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 30 02:25:00 2023
Response via : Initial Calibration

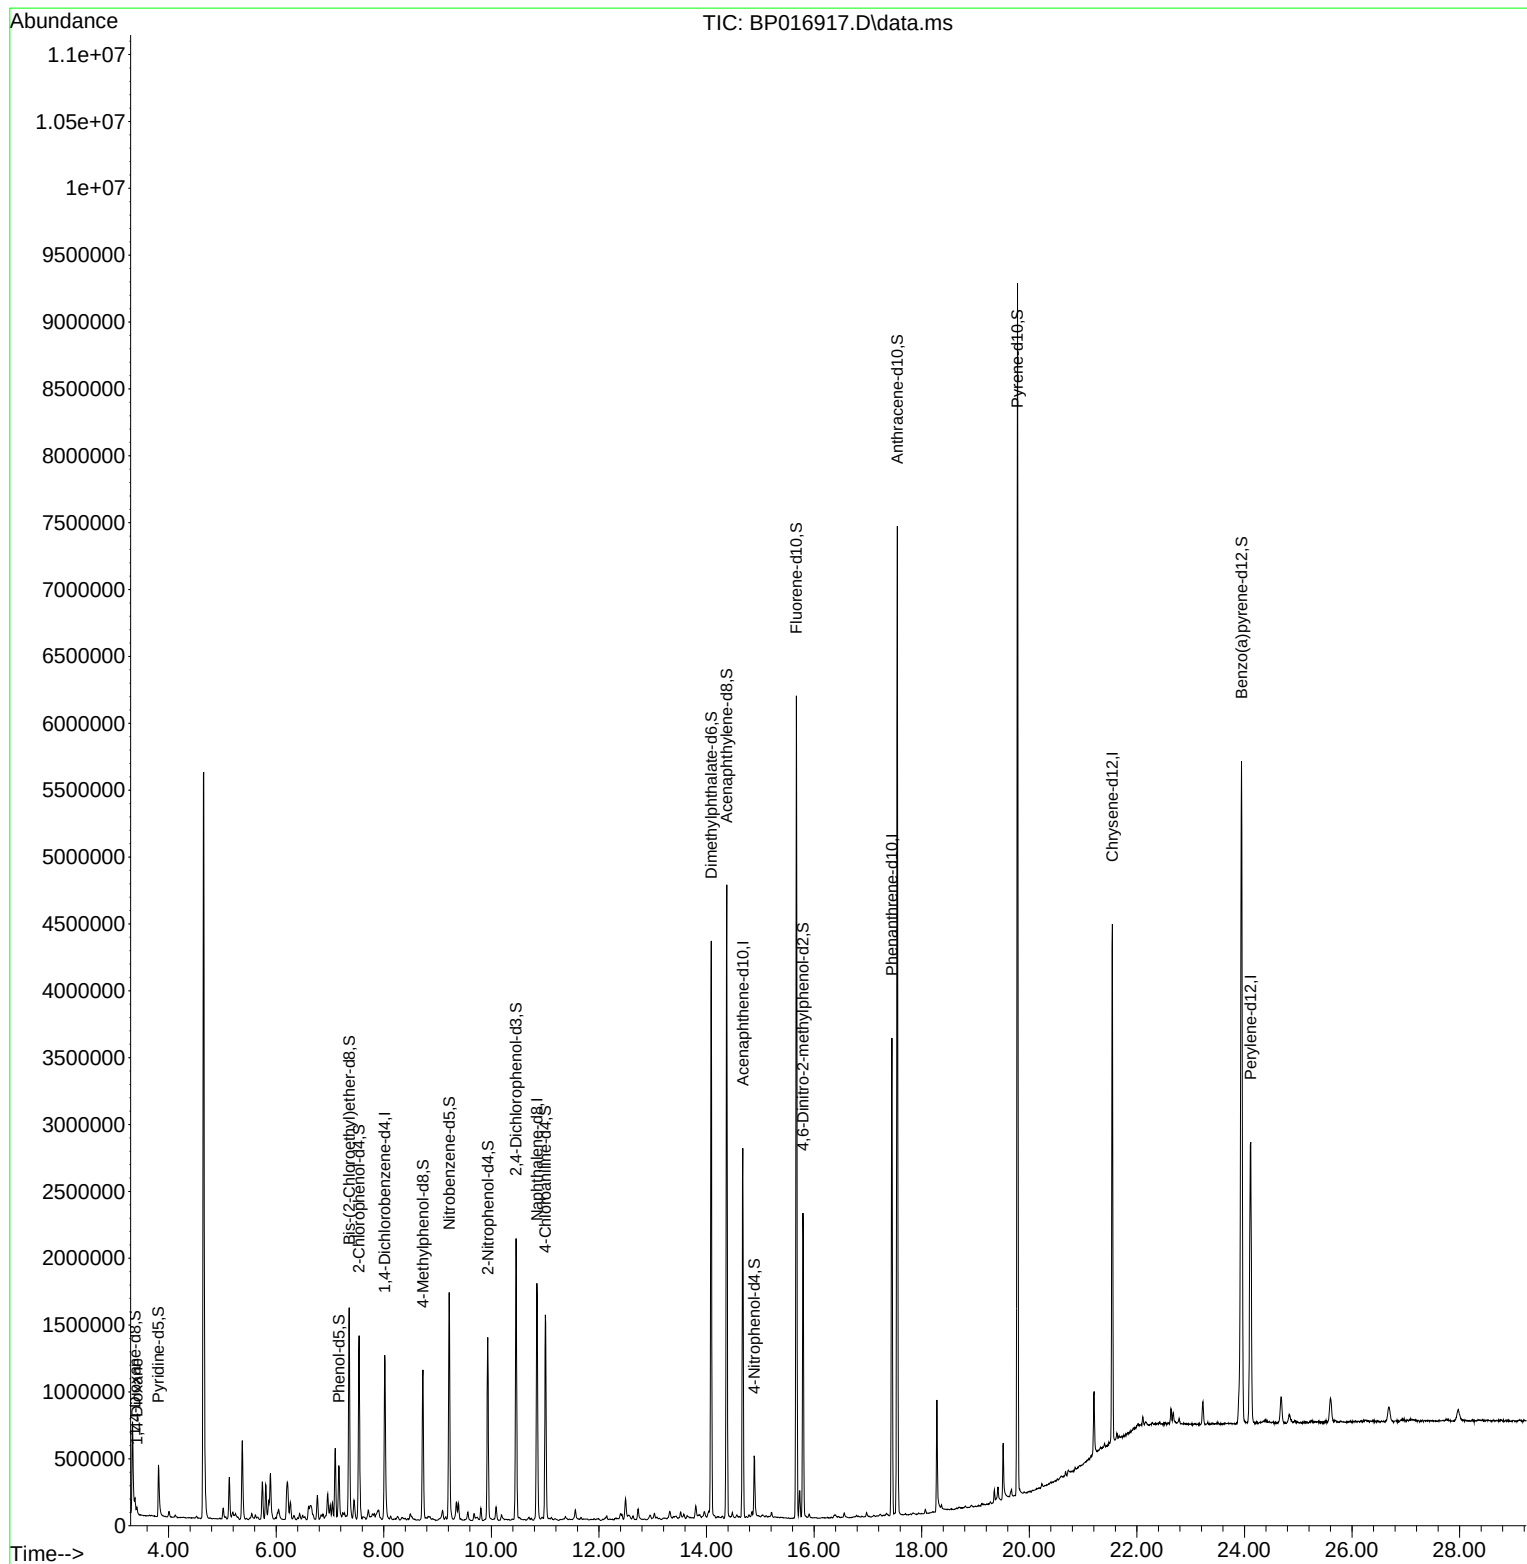

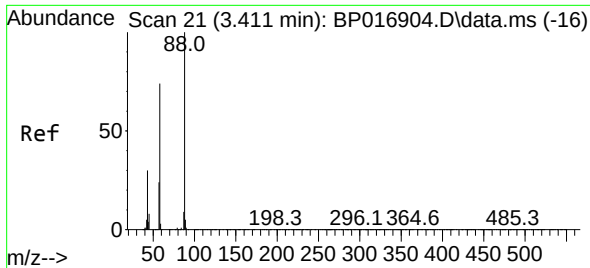

#2
 1,4-Dioxane
 Concen: 2.753 ng/uL
 RT: 3.411 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP016917.D
 Acq: 01 Sep 2023 20:28

Instrument :
 BNA_P
 ClientSampleId :
 BH942

Tgt Ion: 88 Resp: 23239
 Ion Ratio Lower Upper
 88 100
 43 35.3 24.0 36.0
 58 74.8 59.8 89.8

