

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
 Data File : BP016905.D
 Acq On : 01 Sep 2023 13:40
 Operator : MA/JU
 Sample : PB155168BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK168

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016905.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	11	15	27	rVB	227276	309579	2.24%	0.200%
2	3.811	84	89	105	rBV	1940595	2893024	20.93%	1.872%
3	4.122	139	142	148	rVB	42604	59216	0.43%	0.038%
4	7.169	653	660	674	rBV	3078734	4805134	34.76%	3.109%
5	7.358	685	692	702	rVB	2509285	3772165	27.29%	2.441%
6	7.540	715	723	736	rBV	3038619	4726080	34.19%	3.058%
7	8.022	797	805	812	rBV	2212309	3484850	25.21%	2.255%
8	8.728	918	925	937	rBV	3580546	5839935	42.24%	3.779%
9	9.222	1000	1009	1017	rBV	2772994	4590062	33.20%	2.970%
10	9.934	1121	1130	1138	rBV	2416997	3921190	28.37%	2.537%
11	10.457	1211	1219	1233	rBV	3450356	5776790	41.79%	3.738%
12	10.852	1277	1286	1296	rBV	3060308	5138265	37.17%	3.325%
13	11.004	1305	1312	1338	rBV	1494543	2619172	18.95%	1.695%
14	11.599	1409	1413	1422	rVB	6847	14068	0.10%	0.009%
15	12.428	1548	1554	1561	rVB2	58581	95752	0.69%	0.062%
16	13.516	1734	1739	1745	rBV	35771	60266	0.44%	0.039%
17	13.634	1754	1759	1768	rVB3	10790	21325	0.15%	0.014%
18	14.087	1829	1836	1846	rBV	6563312	8795692	63.63%	5.692%
19	14.375	1877	1885	1901	rBV2	7097613	10361758	74.95%	6.705%
20	14.675	1929	1936	1950	rVB	4810814	6833156	49.43%	4.422%
21	14.793	1953	1956	1960	rBV6	9958	14273	0.10%	0.009%
22	14.892	1965	1973	1995	rBV	2860908	4435700	32.09%	2.870%
23	15.675	2098	2106	2113	rBV	8611762	12617919	91.28%	8.165%
24	15.798	2120	2127	2140	rBV	3292833	4399398	31.82%	2.847%
25	15.904	2141	2145	2154	rVB	43277	66369	0.48%	0.043%
26	16.457	2234	2239	2242	rVB6	10908	15057	0.11%	0.010%
27	17.110	2345	2350	2354	rBV8	12248	19774	0.14%	0.013%
28	17.228	2366	2370	2376	rVB2	11453	19492	0.14%	0.013%
29	17.445	2400	2407	2417	rBV	5615170	7675132	55.52%	4.967%
30	17.545	2417	2424	2440	rVV2	9527265	13316810	96.33%	8.617%
31	17.834	2470	2473	2479	rVB2	11643	16843	0.12%	0.011%
32	18.069	2509	2513	2518	rBV7	19636	29208	0.21%	0.019%
33	18.281	2544	2549	2562	rBV	146787	266296	1.93%	0.172%
34	19.351	2727	2731	2736	rBV2	118527	153990	1.11%	0.100%
35	19.416	2739	2742	2752	rVB	100764	176035	1.27%	0.114%
36	19.516	2755	2759	2766	rBV2	157136	248166	1.80%	0.161%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016905.D
Acq On : 01 Sep 2023 13:40
Operator : MA/JU
Sample : PB155168BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK168

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Title : SVOA CALIBRATION

37	19.780	2798	2804	2810	rBV	10881331	13824033	100.00%	8.946%
38	21.545	3098	3104	3112	rBV	4749552	6372010	46.09%	4.123%
39	23.945	3504	3512	3521	rVB2	5474114	10949383	79.21%	7.085%
40	24.110	3533	3540	3550	rVB	2714658	5800000	41.96%	3.753%




Sum of corrected areas: 154533367

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016905.D
Acq On : 01 Sep 2023 13:40
Operator : MA/JU
Sample : PB155168BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK168

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

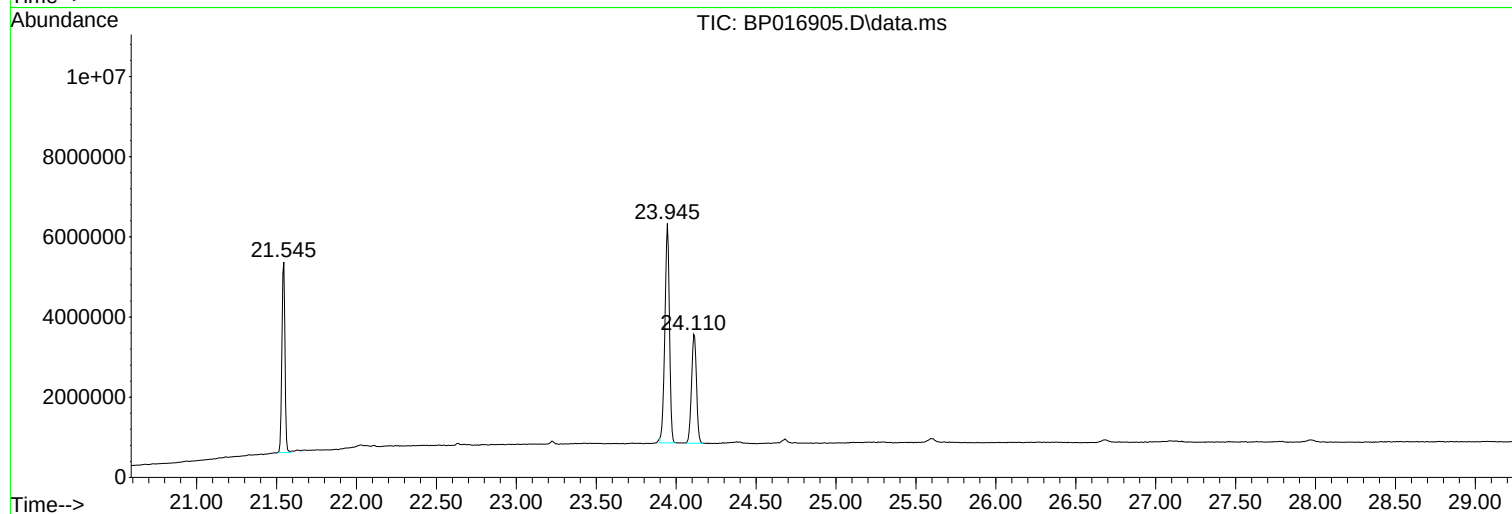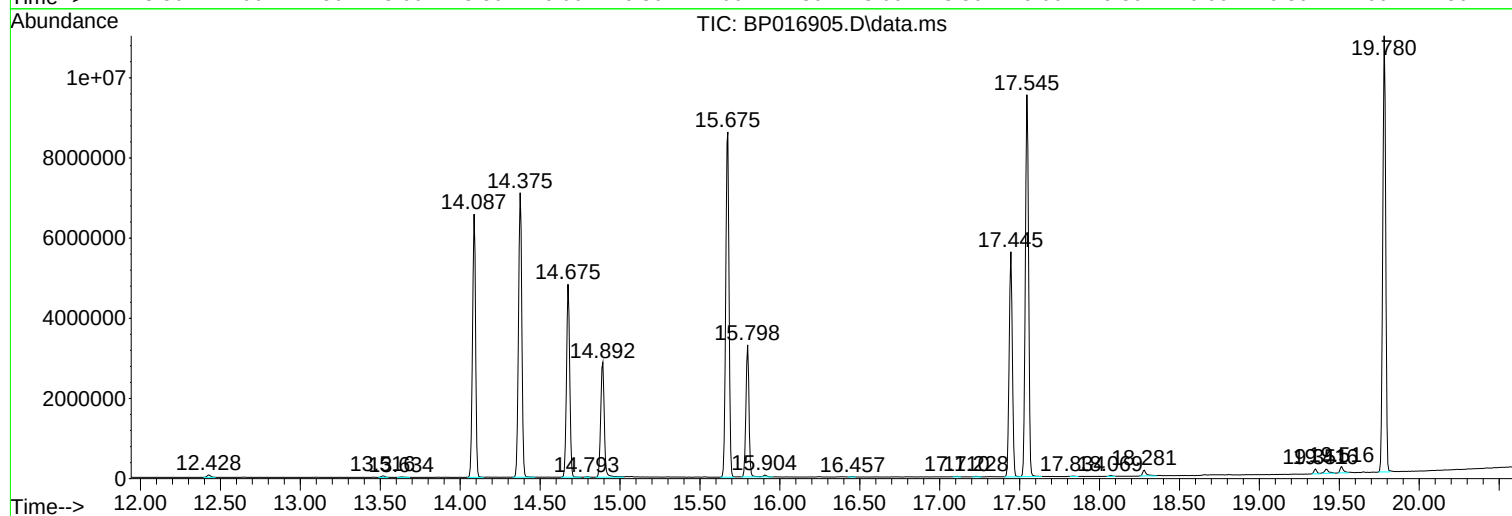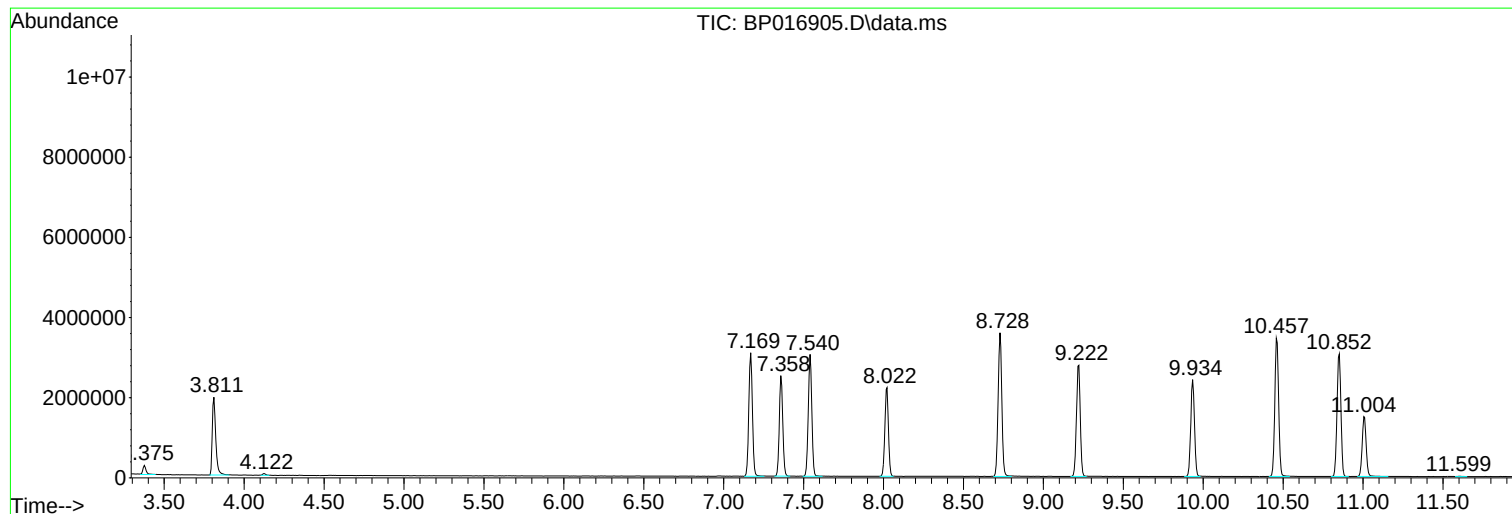

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016905.D
Acq On : 01 Sep 2023 13:40
Operator : MA/JU
Sample : PB155168BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK168

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016905.D
Acq On : 01 Sep 2023 13:40
Operator : MA/JU
Sample : PB155168BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK168

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------