

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
 Data File : BP016916.D
 Acq On : 01 Sep 2023 19:54
 Operator : MA/JU
 Sample : 04123-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH923

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016916.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	11	15	20	rBV	93784	121875	1.09%	0.115%
2	3.811	85	89	104	rBV	621457	988643	8.84%	0.932%
3	4.011	118	123	129	rVB	46410	73455	0.66%	0.069%
4	4.122	139	142	149	rVB	19819	30483	0.27%	0.029%
5	4.652	226	232	244	rVB	389072	624171	5.58%	0.589%
6	5.058	298	301	307	rVB	16881	24202	0.22%	0.023%
7	6.963	622	625	630	rBV5	7636	11700	0.10%	0.011%
8	7.169	652	660	669	rBV	447802	743615	6.65%	0.701%
9	7.357	682	692	708	rBV	1619955	2450119	21.91%	2.310%
10	7.540	716	723	732	rBV	1508584	2400599	21.47%	2.264%
11	7.628	733	738	747	rVB2	11056	26255	0.23%	0.025%
12	8.016	797	804	815	rBV	1386319	2201214	19.69%	2.076%
13	8.728	915	925	937	rBV	1239444	2076202	18.57%	1.958%
14	9.216	1000	1008	1021	rBV	1880790	3047387	27.26%	2.874%
15	9.934	1122	1130	1139	rBV	1507227	2512340	22.47%	2.369%
16	10.457	1209	1219	1234	rBV	2147872	3626346	32.43%	3.420%
17	10.846	1276	1285	1293	rBV	2023789	3373235	30.17%	3.181%
18	11.004	1304	1312	1323	rBV	2089115	3553296	31.78%	3.351%
19	11.593	1408	1412	1418	rBV9	6878	14448	0.13%	0.014%
20	12.428	1548	1554	1566	rVB2	36880	69855	0.62%	0.066%
21	13.516	1734	1739	1745	rBV2	42988	71800	0.64%	0.068%
22	13.639	1755	1760	1764	rVB7	8077	12186	0.11%	0.011%
23	14.087	1829	1836	1843	rBV	4219778	5774177	51.64%	5.445%
24	14.375	1878	1885	1897	rBV	4786034	7079193	63.32%	6.676%
25	14.675	1929	1936	1945	rVB	3164252	4649728	41.59%	4.385%
26	14.792	1951	1956	1964	rBV	7005	13582	0.12%	0.013%
27	14.886	1966	1972	1988	rBV	446660	726852	6.50%	0.685%
28	15.045	1995	1999	2001	rBV5	9587	13558	0.12%	0.013%
29	15.669	2098	2105	2113	rBV	6332481	8753231	78.29%	8.254%
30	15.792	2120	2126	2140	rBV	2206051	2881273	25.77%	2.717%
31	15.904	2141	2145	2150	rVB	27576	39930	0.36%	0.038%
32	16.457	2233	2239	2243	rBV7	9149	14981	0.13%	0.014%
33	17.228	2367	2370	2376	rVB2	9648	15486	0.14%	0.015%
34	17.445	2400	2407	2416	rBV	3904918	5645420	50.49%	5.324%
35	17.545	2417	2424	2436	rBV	7096634	9683702	86.61%	9.132%
36	18.069	2509	2513	2521	rVB10	18056	29741	0.27%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016916.D
Acq On : 01 Sep 2023 19:54
Operator : MA/JU
Sample : 04123-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH923

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Title : SVOA CALIBRATION

37	18.280	2544	2549	2560	rBV	265536	431718	3.86%	0.407%
38	18.369	2562	2564	2568	rVB2	18095	19846	0.18%	0.019%
39	19.351	2727	2731	2734	rBV	90928	117502	1.05%	0.111%
40	19.416	2739	2742	2751	rVB	90005	146653	1.31%	0.138%
41	19.516	2755	2759	2770	rBV	191092	333157	2.98%	0.314%
42	19.651	2779	2782	2786	rBV3	37658	45755	0.41%	0.043%
43	19.780	2798	2804	2810	rBV	8769769	11180827	100.00%	10.544%
44	21.545	3098	3104	3109	rBV	4235156	5645093	50.49%	5.323%
45	23.945	3504	3512	3522	rVB2	4634820	9601839	85.88%	9.055%
46	24.110	3533	3540	3551	rVB	2478597	5147006	46.03%	4.854%




Sum of corrected areas: 106043676

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016916.D
Acq On : 01 Sep 2023 19:54
Operator : MA/JU
Sample : 04123-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH923

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

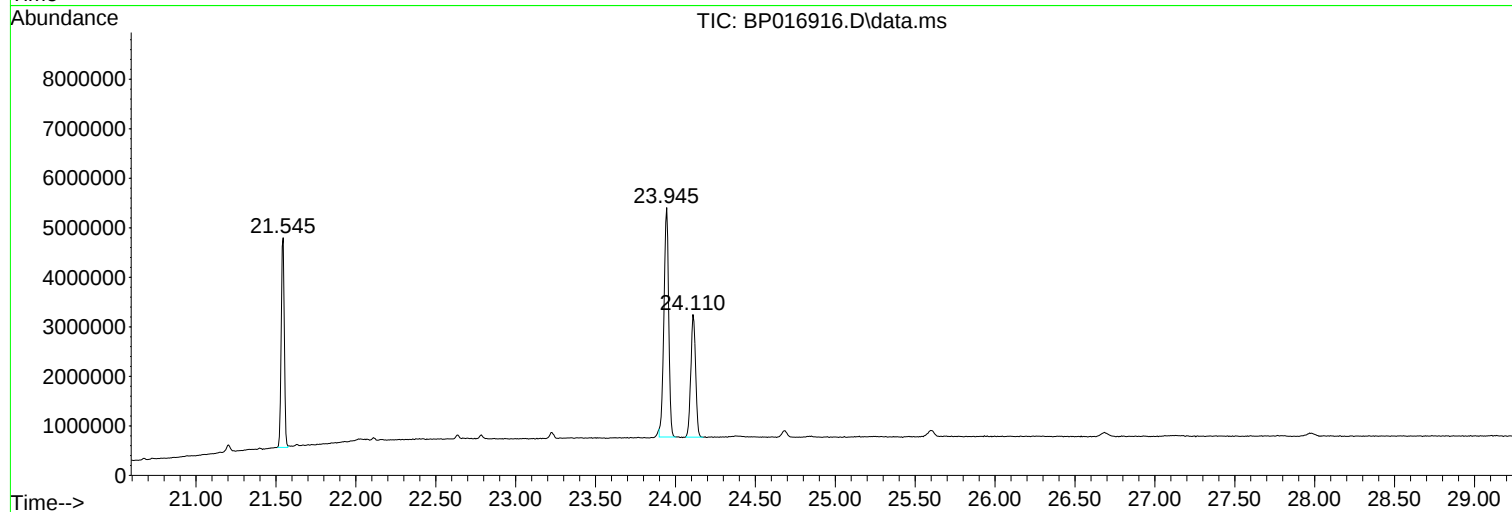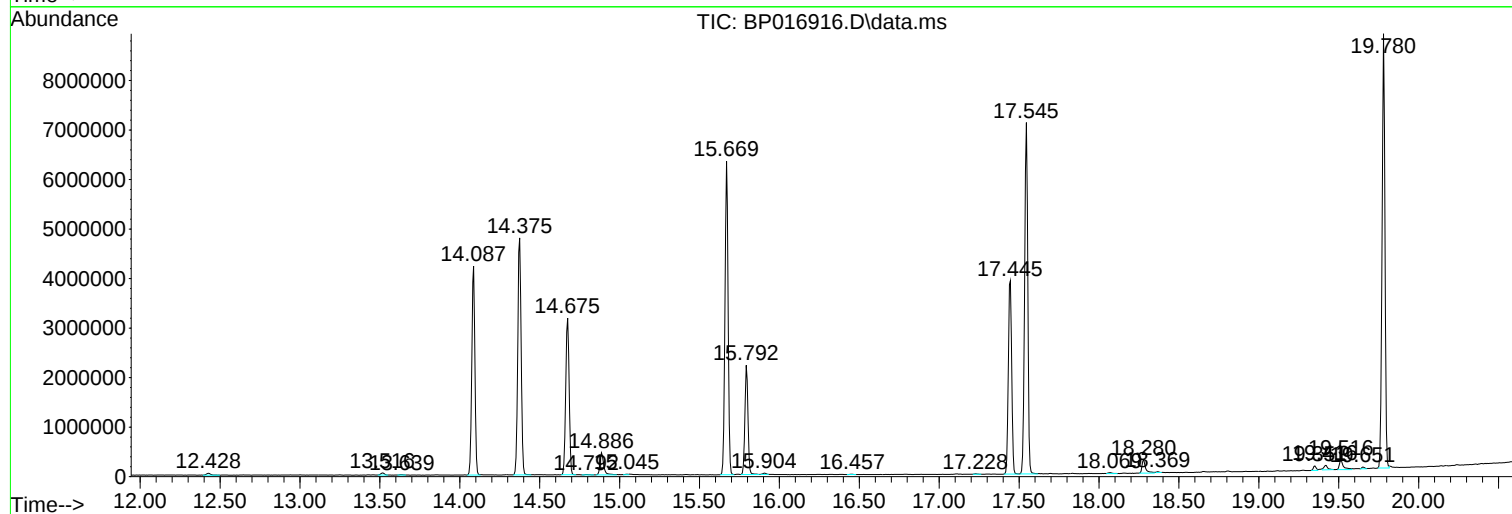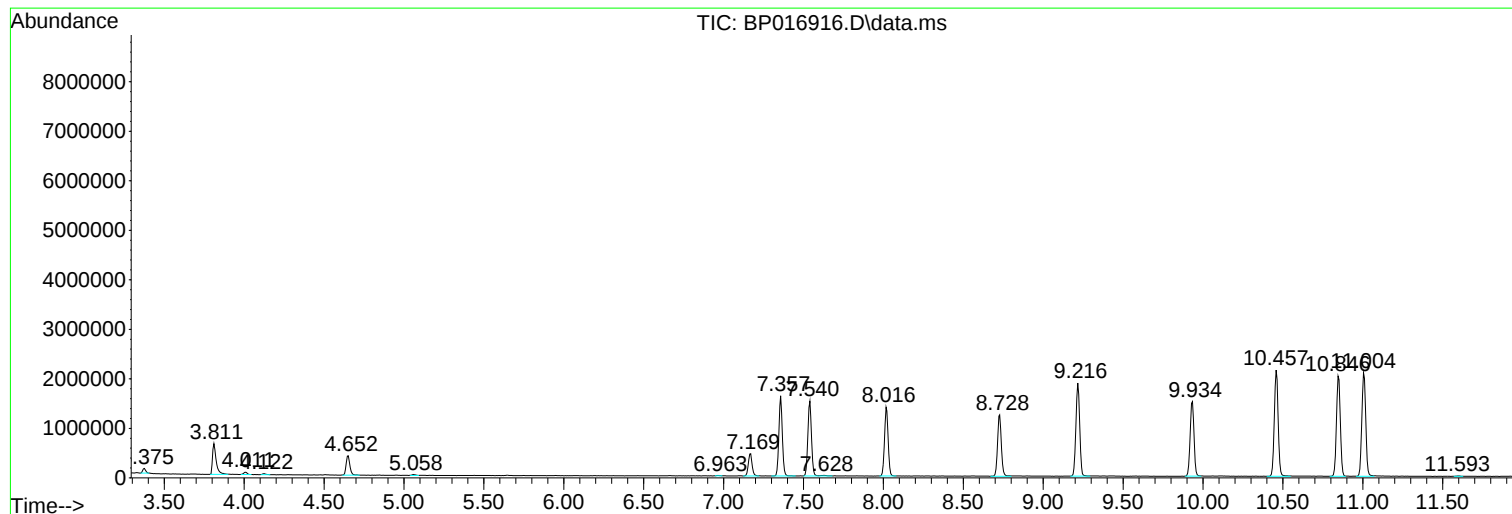

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016916.D
Acq On : 01 Sep 2023 19:54
Operator : MA/JU
Sample : 04123-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH923










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.652	5.67 ng/ul	624171	1,4-Dichlorobenzene-d4	8.016

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	38

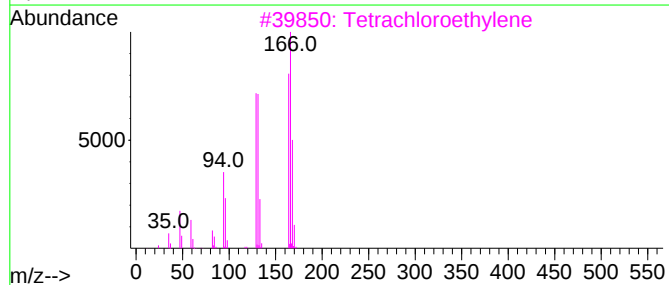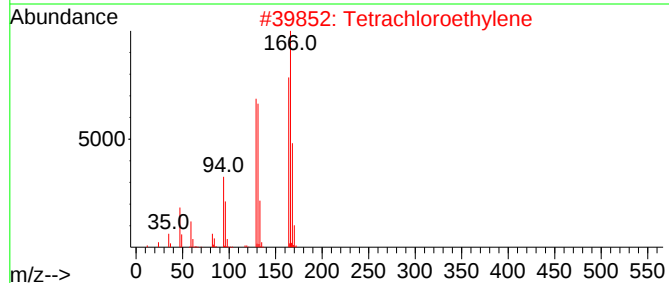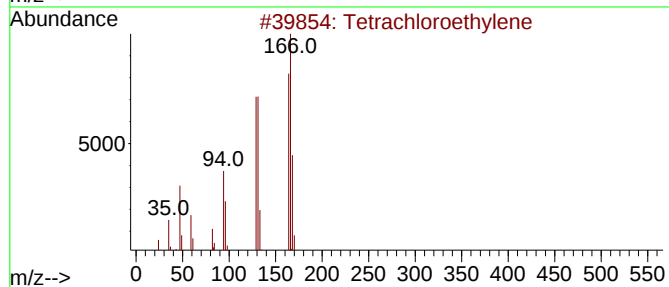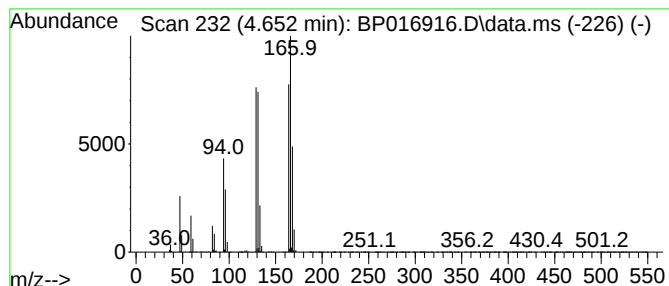

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016916.D
Acq On : 01 Sep 2023 19:54
Operator : MA/JU
Sample : 04123-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH923

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.652	5.7	ng/u1	624171	1	8.016	2201210	20.0