

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
 Data File : BP016919.D
 Acq On : 01 Sep 2023 21:35
 Operator : MA/JU
 Sample : 04123-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAA8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016919.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.376	11	15	26	rVB	100514	165969	1.45%	0.159%
2	3.811	85	89	105	rBV	632705	1006908	8.79%	0.962%
3	4.005	118	122	129	rVB	53283	81005	0.71%	0.077%
4	4.123	138	142	151	rVB	35791	56597	0.49%	0.054%
5	4.511	205	208	215	rVB6	12970	17497	0.15%	0.017%
6	4.646	227	231	239	rVB3	20050	34016	0.30%	0.033%
7	5.058	298	301	306	rVB	18150	26647	0.23%	0.025%
8	7.164	653	659	670	rBV	471469	753449	6.58%	0.720%
9	7.358	685	692	702	rBV	1635003	2521249	22.01%	2.409%
10	7.540	715	723	733	rBV	1565321	2517975	21.98%	2.406%
11	8.017	796	804	819	rBV	1229776	1932431	16.87%	1.846%
12	8.722	917	924	938	rBV	1324157	2155699	18.82%	2.060%
13	9.216	1000	1008	1025	rBV	1978088	3207693	28.00%	3.065%
14	9.428	1040	1044	1050	rVB5	6224	11487	0.10%	0.011%
15	9.928	1120	1129	1143	rBV	1589429	2645958	23.10%	2.528%
16	10.458	1210	1219	1234	rBV	2366745	3919995	34.22%	3.746%
17	10.846	1277	1285	1293	rBV	1806375	2982949	26.04%	2.850%
18	11.005	1304	1312	1325	rBV	2042247	3368398	29.41%	3.219%
19	11.587	1406	1411	1415	rBV8	6168	12672	0.11%	0.012%
20	11.663	1420	1424	1432	rVB9	8144	15546	0.14%	0.015%
21	11.922	1464	1468	1474	rVB3	12537	20741	0.18%	0.020%
22	12.428	1546	1554	1564	rVB2	40622	71494	0.62%	0.068%
23	13.516	1732	1739	1744	rBV	46297	73304	0.64%	0.070%
24	13.916	1801	1807	1813	rVB4	7773	11885	0.10%	0.011%
25	14.087	1829	1836	1847	rVV	4593717	6249686	54.56%	5.972%
26	14.375	1877	1885	1899	rBV	5151445	7632026	66.63%	7.292%
27	14.581	1915	1920	1926	rBV2	7364	12946	0.11%	0.012%
28	14.675	1927	1936	1944	rVB	2833848	4171154	36.41%	3.986%
29	14.793	1952	1956	1960	rBV7	9335	16046	0.14%	0.015%
30	14.887	1966	1972	1988	rBV	423125	684757	5.98%	0.654%
31	15.481	2066	2073	2077	rVB2	8663	14637	0.13%	0.014%
32	15.669	2098	2105	2111	rBV	6825919	9427367	82.30%	9.008%
33	15.728	2111	2115	2120	rVV	212290	310335	2.71%	0.297%
34	15.793	2120	2126	2139	rVV	2277139	3056374	26.68%	2.920%
35	15.898	2139	2144	2151	rVB3	67531	111358	0.97%	0.106%
36	16.387	2222	2227	2234	rBV5	11071	22817	0.20%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
 Data File : BP016919.D
 Acq On : 01 Sep 2023 21:35
 Operator : MA/JU
 Sample : 04123-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAA8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

37	17.110	2345	2350	2355	rVB9	9030	17620	0.15%	0.017%
38	17.228	2365	2370	2378	rBV5	11153	22882	0.20%	0.022%
39	17.440	2400	2406	2416	rBV	3516744	5019313	43.82%	4.796%
40	17.545	2417	2424	2436	rBV	7357153	10327634	90.16%	9.868%
41	17.834	2470	2473	2477	rBV3	9774	11908	0.10%	0.011%
42	18.063	2509	2512	2519	rVB9	13785	19966	0.17%	0.019%
43	18.275	2544	2548	2557	rBV	161021	251612	2.20%	0.240%
44	18.369	2561	2564	2567	rVB	14388	17809	0.16%	0.017%
45	19.345	2727	2730	2735	rBV	89005	121209	1.06%	0.116%
46	19.416	2738	2742	2747	rVB	81536	114640	1.00%	0.110%
47	19.510	2754	2758	2765	rBV2	120410	176202	1.54%	0.168%
48	19.781	2798	2804	2809	rBV	8714979	11455046	100.00%	10.945%
49	21.539	3098	3103	3110	rBV2	3535976	4639094	40.50%	4.433%
50	23.939	3504	3511	3525	rVB2	4294158	9080727	79.27%	8.677%
51	24.110	3533	3540	3551	rVB	1890438	4059779	35.44%	3.879%




Sum of corrected areas: 104656508

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016919.D
Acq On : 01 Sep 2023 21:35
Operator : MA/JU
Sample : 04123-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAA8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

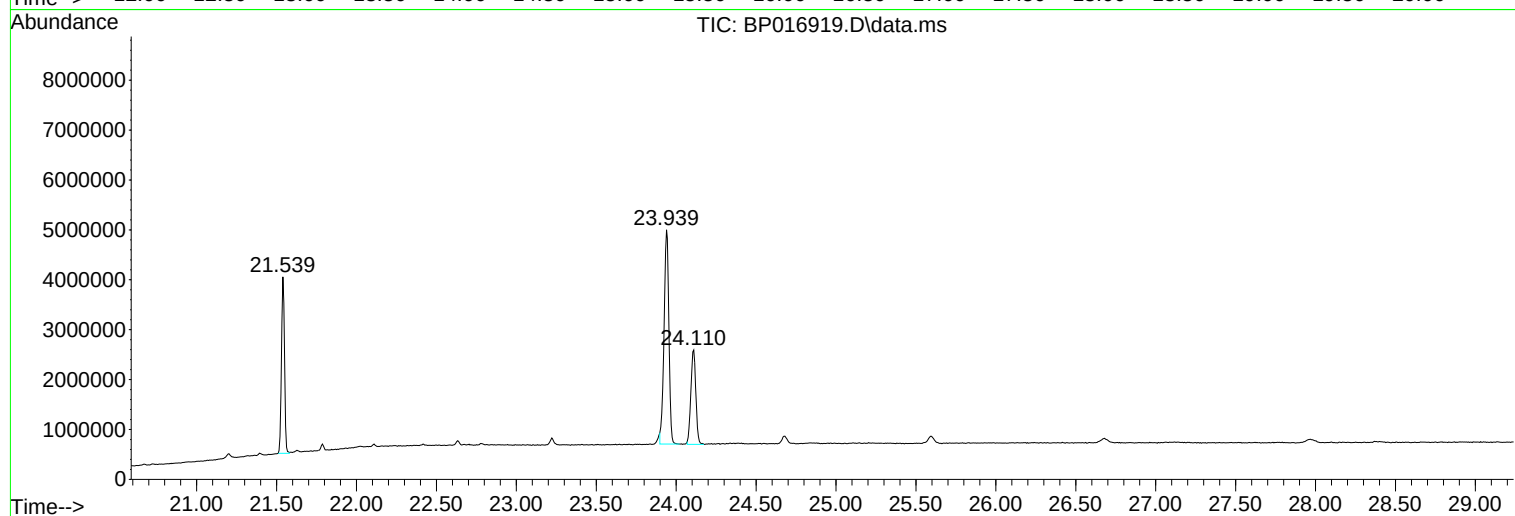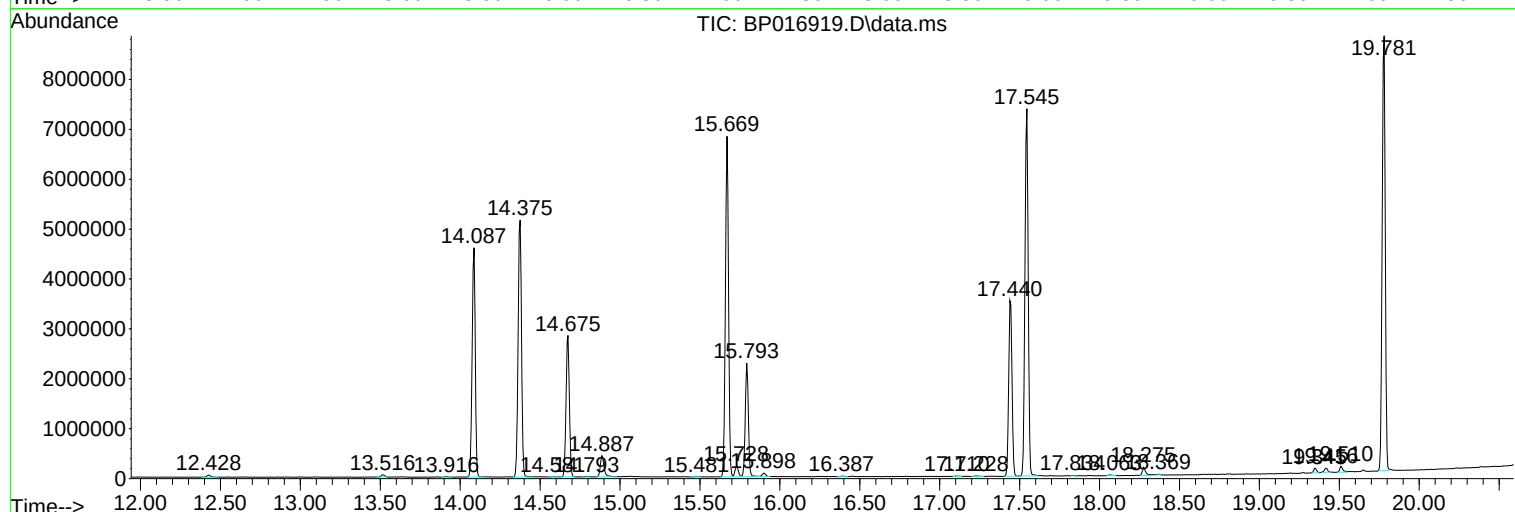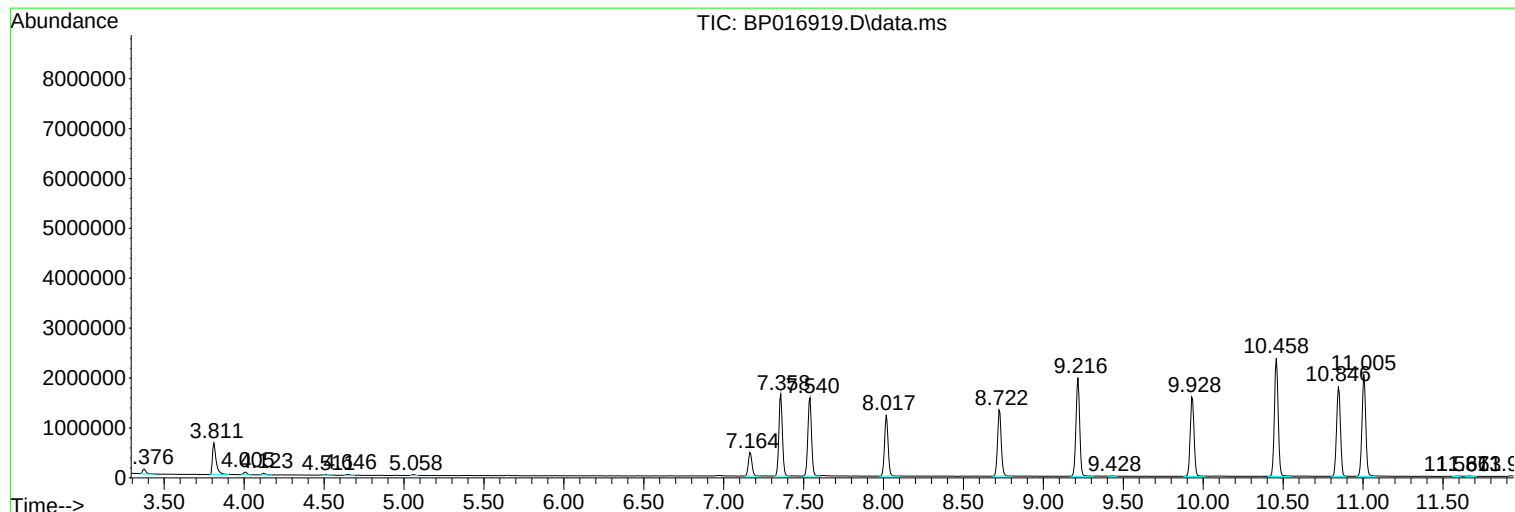

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016919.D
Acq On : 01 Sep 2023 21:35
Operator : MA/JU
Sample : 04123-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAA8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016919.D
Acq On : 01 Sep 2023 21:35
Operator : MA/JU
Sample : 04123-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAA8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------