

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
 Data File : BP016923.D
 Acq On : 02 Sep 2023 00:25
 Operator : MA/JU
 Sample : PB155234BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK234

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016923.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	11	15	25	rVB	114871	174971	1.59%	0.161%
2	3.810	85	89	111	rBV	1070322	1732514	15.74%	1.590%
3	4.116	138	141	148	rBV	22325	36871	0.33%	0.034%
4	7.163	652	659	671	rBV	1797176	2878512	26.15%	2.642%
5	7.357	682	692	706	rVB	1481684	2280413	20.71%	2.093%
6	7.540	715	723	736	rBV	1734701	2790441	25.35%	2.561%
7	8.016	797	804	819	rBV	1321818	2085914	18.95%	1.915%
8	8.722	917	924	936	rBV	2192365	3649381	33.15%	3.350%
9	9.216	1001	1008	1017	rBV	1743048	2847217	25.86%	2.614%
10	9.928	1122	1129	1144	rBV	1463574	2450588	22.26%	2.250%
11	10.457	1210	1219	1232	rBV	2276858	3730701	33.89%	3.425%
12	10.845	1277	1285	1294	rVB	2029035	3294325	29.92%	3.024%
13	11.004	1304	1312	1329	rBV	1074650	1859085	16.89%	1.707%
14	11.592	1406	1412	1418	rBV	5389	11024	0.10%	0.010%
15	12.428	1548	1554	1559	rBV	36875	58855	0.53%	0.054%
16	13.516	1734	1739	1744	rBV2	36536	55506	0.50%	0.051%
17	14.086	1829	1836	1847	rBV	4360928	5934681	53.90%	5.448%
18	14.374	1877	1885	1899	rBV	4753215	7057437	64.10%	6.478%
19	14.674	1927	1936	1949	rVB	3257538	4802018	43.62%	4.408%
20	14.886	1964	1972	1993	rBV	2177394	3288909	29.87%	3.019%
21	15.669	2098	2105	2113	rBV	6446103	8781911	79.76%	8.061%
22	15.792	2119	2126	2138	rBV	2146103	2867392	26.04%	2.632%
23	15.904	2141	2145	2152	rVB2	29878	43869	0.40%	0.040%
24	16.451	2235	2238	2242	rBV6	6898	11578	0.11%	0.011%
25	17.110	2346	2350	2355	rVB7	7713	11914	0.11%	0.011%
26	17.227	2365	2370	2375	rBV3	10463	19076	0.17%	0.018%
27	17.439	2399	2406	2416	rBV	4224812	5915386	53.73%	5.430%
28	17.539	2417	2423	2439	rVB	6810032	9753302	88.59%	8.953%
29	18.274	2544	2548	2555	rBV4	35431	58489	0.53%	0.054%
30	19.345	2726	2730	2735	rBV	88258	118503	1.08%	0.109%
31	19.415	2738	2742	2746	rVV	84776	109731	1.00%	0.101%
32	19.509	2755	2758	2762	rBV4	38573	54480	0.49%	0.050%
33	19.651	2779	2782	2786	rVB3	32132	30999	0.28%	0.028%
34	19.774	2797	2803	2809	rBV	8236166	11009747	100.00%	10.106%
35	21.539	3098	3103	3110	rBV	4260617	5560816	50.51%	5.105%
36	23.933	3503	3510	3521	rVB2	4143658	8727223	79.27%	8.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016923.D
Acq On : 02 Sep 2023 00:25
Operator : MA/JU
Sample : PB155234BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK234

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Title : SVOA CALIBRATION

37	24.103	3532	3539	3550	rVB	2236437	4845041	44.01%	4.447%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 108938820

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016923.D
Acq On : 02 Sep 2023 00:25
Operator : MA/JU
Sample : PB155234BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK234

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

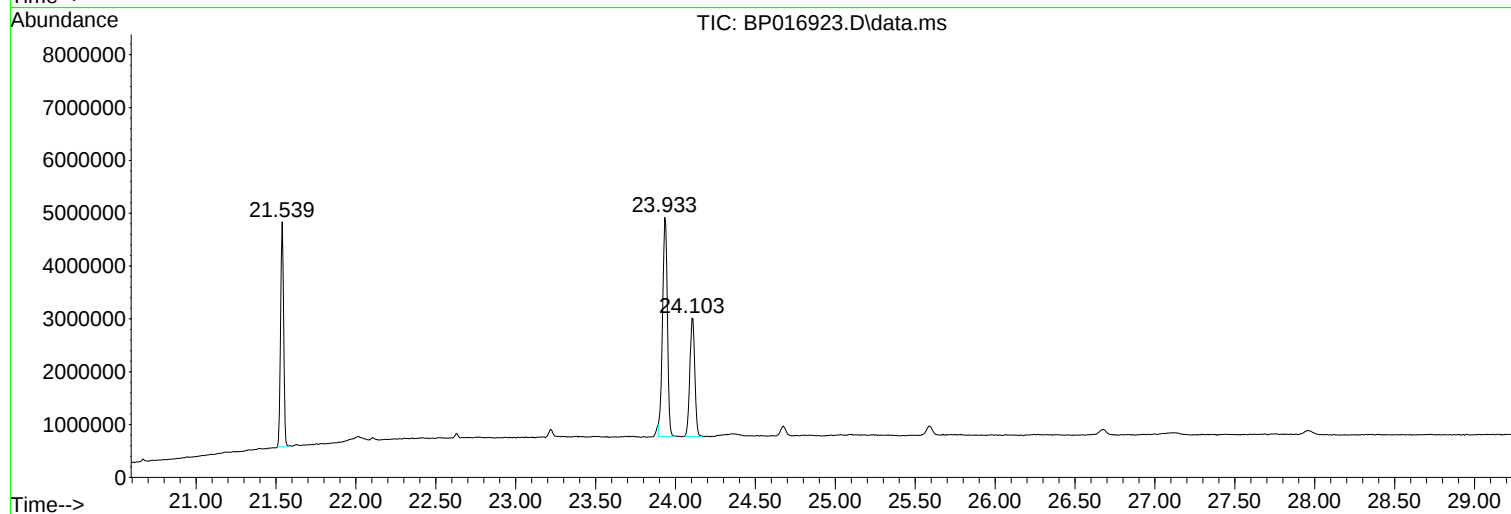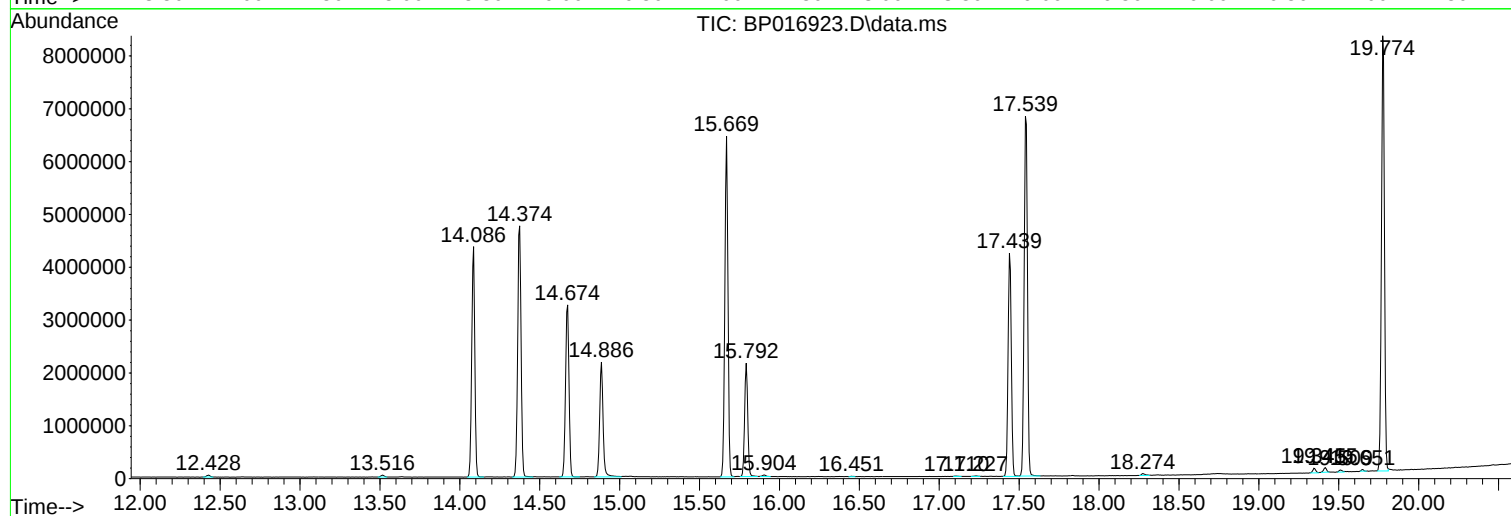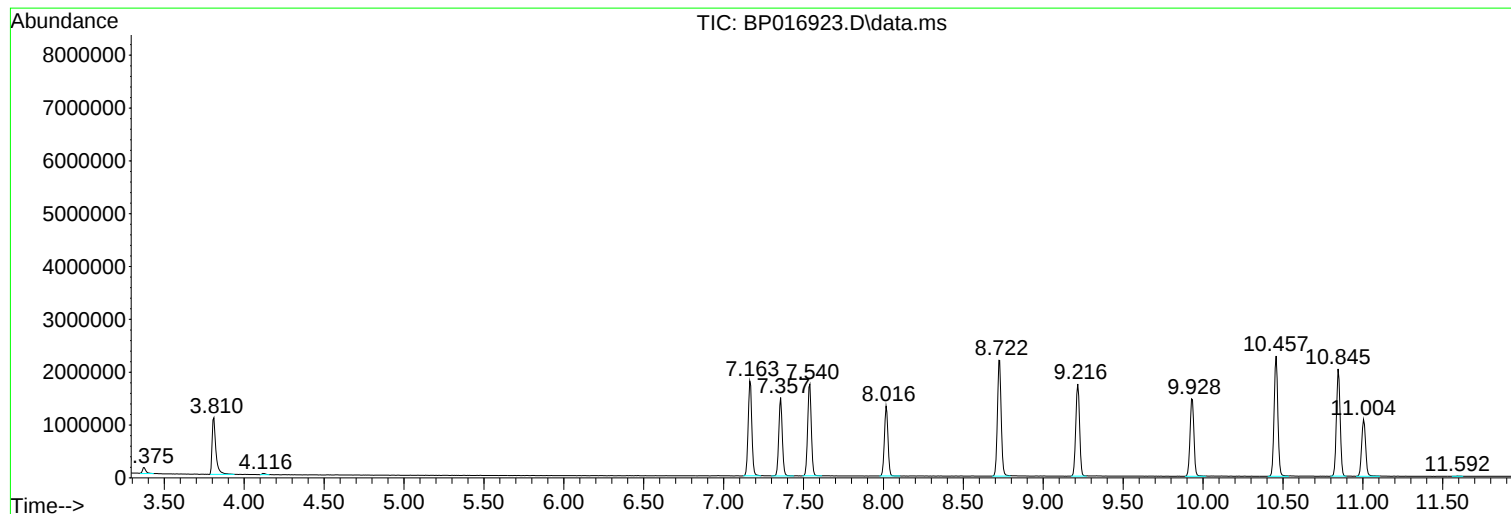

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016923.D
Acq On : 02 Sep 2023 00:25
Operator : MA/JU
Sample : PB155234BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK234

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016923.D
Acq On : 02 Sep 2023 00:25
Operator : MA/JU
Sample : PB155234BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK234

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------