

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
 Data File : BP016924.D
 Acq On : 02 Sep 2023 00:58
 Operator : MA/JU
 Sample : PB155236BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK236

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016924.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	10	14	24	rVB	141636	219065	1.90%	0.193%
2	3.805	84	88	106	rBV	1582060	2528951	21.97%	2.225%
3	4.122	138	142	147	rBV	18941	24844	0.22%	0.022%
4	7.163	652	659	671	rBV	1956437	3081961	26.78%	2.712%
5	7.358	684	692	701	rBV	1539323	2402699	20.87%	2.114%
6	7.540	714	723	730	rBV	1839432	2976952	25.86%	2.619%
7	8.016	797	804	815	rBV	1324211	2065393	17.94%	1.817%
8	8.722	916	924	940	rBV	2328724	3849275	33.44%	3.387%
9	9.216	1000	1008	1016	rBV	1841881	2999958	26.06%	2.639%
10	9.928	1119	1129	1145	rBV	1554581	2583315	22.44%	2.273%
11	10.457	1210	1219	1232	rBV	2325697	3876743	33.68%	3.411%
12	10.846	1278	1285	1293	rBV	1926928	3185553	27.68%	2.803%
13	11.004	1301	1312	1331	rBV	2338612	3913239	34.00%	3.443%
14	12.422	1548	1553	1562	rVB	38942	68825	0.60%	0.061%
15	13.516	1732	1739	1747	rVB	36440	60221	0.52%	0.053%
16	13.634	1753	1759	1767	rBV6	6807	14183	0.12%	0.012%
17	14.087	1829	1836	1849	rBV	4233775	5946704	51.66%	5.232%
18	14.375	1877	1885	1901	rBV	4830418	7161842	62.22%	6.301%
19	14.675	1928	1936	1943	rBV	2984002	4434874	38.53%	3.902%
20	14.887	1965	1972	1991	rBV	2332381	3431169	29.81%	3.019%
21	15.063	2000	2002	2007	rVB6	8366	12100	0.11%	0.011%
22	15.669	2098	2105	2114	rBV	6345817	8825246	76.67%	7.765%
23	15.792	2120	2126	2134	rBV	2211220	2884480	25.06%	2.538%
24	15.904	2140	2145	2150	rVB3	28504	39337	0.34%	0.035%
25	17.104	2345	2349	2353	rVB6	9693	14321	0.12%	0.013%
26	17.222	2366	2369	2376	rBV4	8914	14872	0.13%	0.013%
27	17.439	2399	2406	2414	rBV	3908463	5431937	47.19%	4.779%
28	17.539	2417	2423	2437	rVV2	6937085	9924745	86.22%	8.732%
29	18.275	2544	2548	2559	rBV7	28351	54256	0.47%	0.048%
30	19.345	2726	2730	2735	rBV	89516	124626	1.08%	0.110%
31	19.416	2738	2742	2751	rVB	81603	116816	1.01%	0.103%
32	19.510	2755	2758	2763	rBV7	27151	42283	0.37%	0.037%
33	19.775	2797	2803	2817	rBV	8832154	11510442	100.00%	10.127%
34	21.539	3097	3103	3110	rBV	4007083	5414146	47.04%	4.764%
35	23.933	3503	3510	3525	rVB2	4583155	9674038	84.05%	8.512%
36	24.104	3532	3539	3551	rVB	2267414	4747878	41.25%	4.177%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016924.D
Acq On : 02 Sep 2023 00:58
Operator : MA/JU
Sample : PB155236BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK236

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 113657289

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016924.D
Acq On : 02 Sep 2023 00:58
Operator : MA/JU
Sample : PB155236BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK236

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

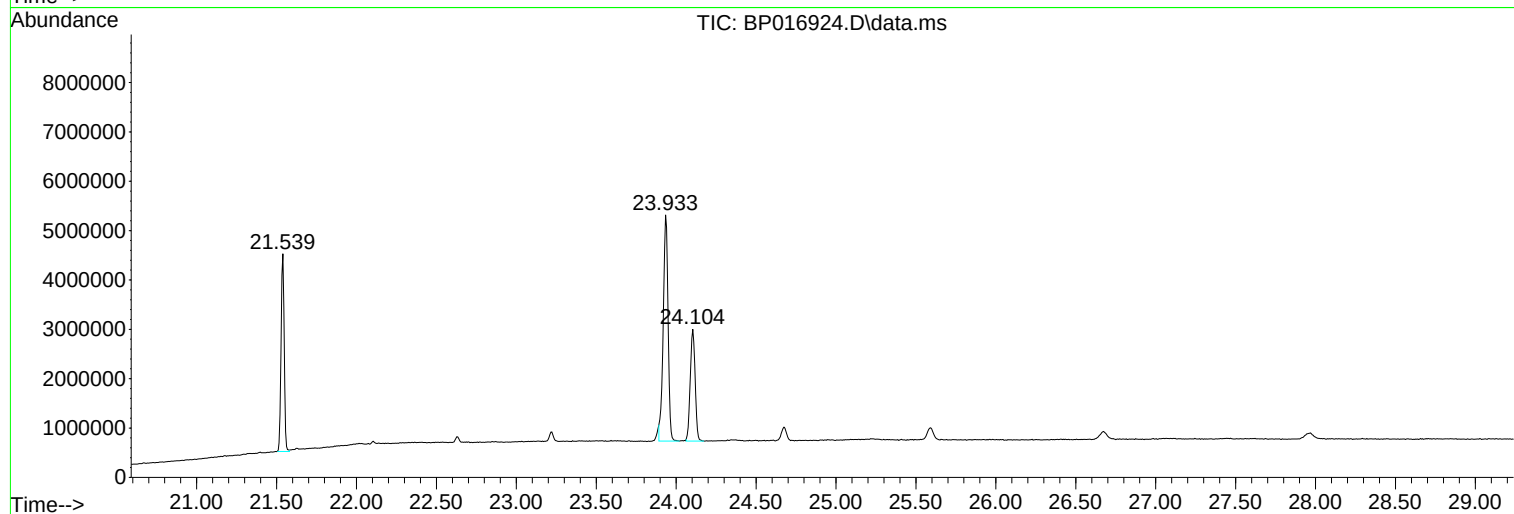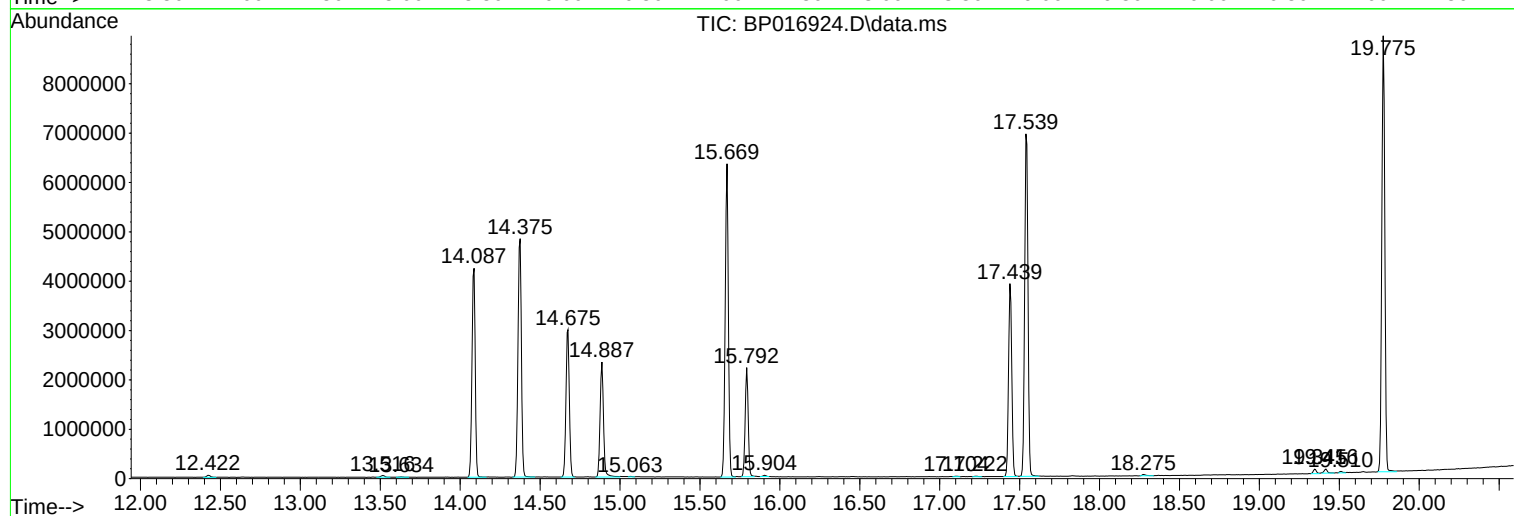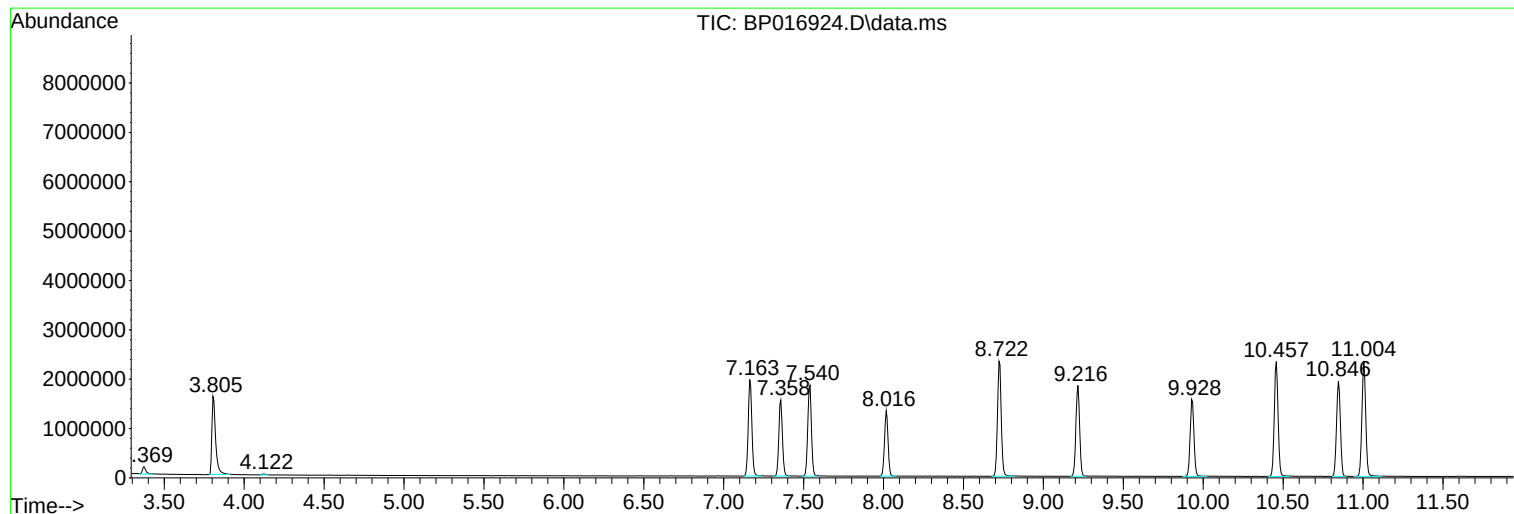

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016924.D
Acq On : 02 Sep 2023 00:58
Operator : MA/JU
Sample : PB155236BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK236

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016924.D
Acq On : 02 Sep 2023 00:58
Operator : MA/JU
Sample : PB155236BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK236

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------