

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
 Data File : BP016929.D
 Acq On : 02 Sep 2023 03:48
 Operator : MA/JU
 Sample : 04209-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH467

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016929.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	11	14	26	rVB	72878	116285	0.93%	0.110%
2	3.811	85	89	108	rVB	439089	731050	5.85%	0.690%
3	4.005	117	122	130	rVB	37867	64037	0.51%	0.060%
4	4.123	138	142	148	rBV	16470	25262	0.20%	0.024%
5	5.058	298	301	306	rVB	11839	15928	0.13%	0.015%
6	6.964	620	625	628	rBV5	6731	12678	0.10%	0.012%
7	7.164	652	659	670	rVB	325465	520037	4.16%	0.491%
8	7.352	683	691	701	rBV	1403396	2197132	17.59%	2.074%
9	7.534	715	722	733	rBV	1252067	1966499	15.74%	1.856%
10	8.016	796	804	817	rVB	1164616	1826802	14.62%	1.724%
11	8.722	917	924	934	rBV	1001980	1612800	12.91%	1.522%
12	9.216	999	1008	1018	rBV	1701021	2810701	22.50%	2.653%
13	9.422	1039	1043	1048	rVB4	8434	14820	0.12%	0.014%
14	9.928	1121	1129	1141	rBV	1397178	2258053	18.08%	2.131%
15	10.458	1211	1219	1232	rBV	1942480	3255381	26.06%	3.072%
16	10.846	1276	1285	1296	rBV	1786444	2965112	23.74%	2.798%
17	11.005	1303	1312	1324	rBV	2053464	3429960	27.46%	3.237%
18	11.593	1406	1412	1417	rBV7	9649	17684	0.14%	0.017%
19	12.422	1546	1553	1561	rBV	36941	63324	0.51%	0.060%
20	13.428	1718	1724	1727	rBV3	11423	17033	0.14%	0.016%
21	13.510	1732	1738	1744	rBV3	21301	36281	0.29%	0.034%
22	13.628	1752	1758	1764	rVB5	6730	14183	0.11%	0.013%
23	14.081	1829	1835	1848	rBV	4323111	5959012	47.70%	5.624%
24	14.369	1876	1884	1895	rBV	4760722	7092553	56.78%	6.694%
25	14.669	1926	1935	1943	rBV	2903597	4352284	34.84%	4.108%
26	14.887	1966	1972	1986	rBV	326576	570844	4.57%	0.539%
27	15.104	2006	2009	2013	rVB5	10384	14902	0.12%	0.014%
28	15.669	2096	2105	2113	rBV	6528498	9109018	72.92%	8.597%
29	15.793	2119	2126	2139	rBV	2257160	2954712	23.65%	2.789%
30	15.904	2141	2145	2151	rVB	28924	42949	0.34%	0.041%
31	16.387	2222	2227	2232	rVV2	7529	14455	0.12%	0.014%
32	17.104	2346	2349	2355	rVB7	8582	13408	0.11%	0.013%
33	17.228	2366	2370	2378	rVB5	10180	23393	0.19%	0.022%
34	17.439	2399	2406	2415	rBV	3971934	5478723	43.86%	5.171%
35	17.539	2416	2423	2435	rVV2	7373687	10657126	85.31%	10.058%
36	17.616	2435	2436	2444	rVB8	12541	19505	0.16%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016929.D
Acq On : 02 Sep 2023 03:48
Operator : MA/JU
Sample : 04209-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH467

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Title : SVOA CALIBRATION

37	18.275	2543	2548	2556	rBV	202339	300426	2.40%	0.284%
38	19.345	2726	2730	2735	rBV	92071	116002	0.93%	0.109%
39	19.416	2738	2742	2751	rVB	94756	126910	1.02%	0.120%
40	19.510	2754	2758	2765	rBV	135492	194838	1.56%	0.184%
41	19.645	2779	2781	2785	rVB2	30608	32412	0.26%	0.031%
42	19.775	2797	2803	2809	rBV	9606383	12491958	100.00%	11.790%
43	21.539	3098	3103	3110	rBV	4514378	5694417	45.58%	5.374%
44	23.933	3503	3510	3522	rVB2	5346812	11324705	90.66%	10.688%
45	24.104	3532	3539	3552	rVB	2535455	5398574	43.22%	5.095%




Sum of corrected areas: 105954168

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016929.D
Acq On : 02 Sep 2023 03:48
Operator : MA/JU
Sample : 04209-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH467

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

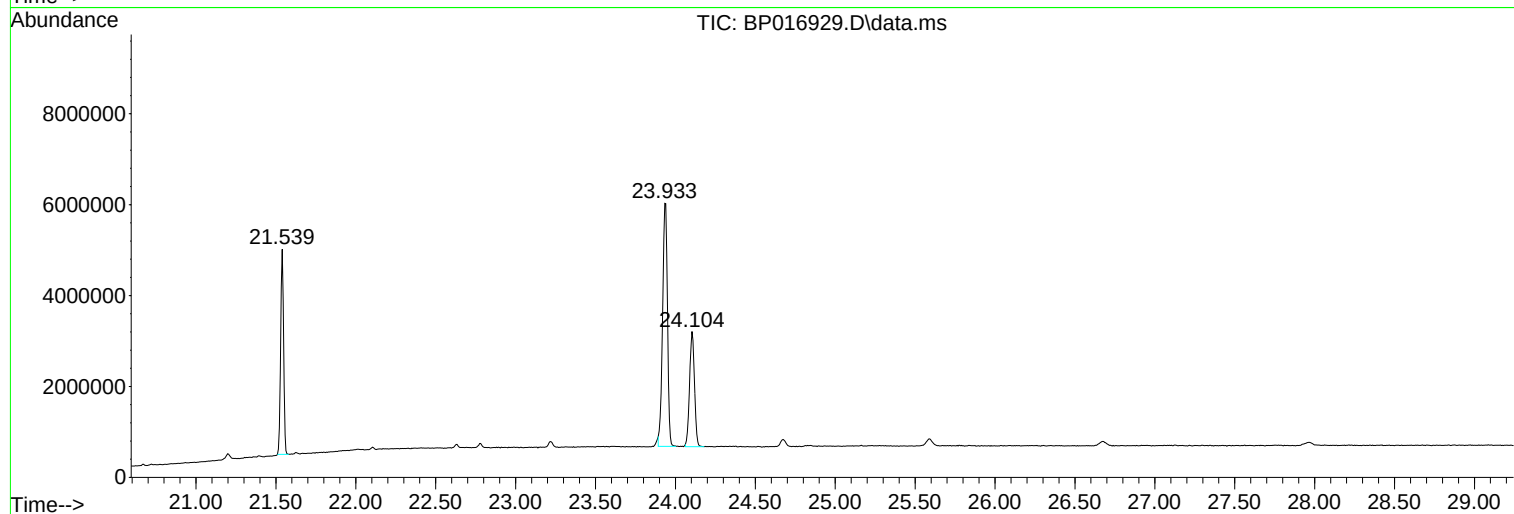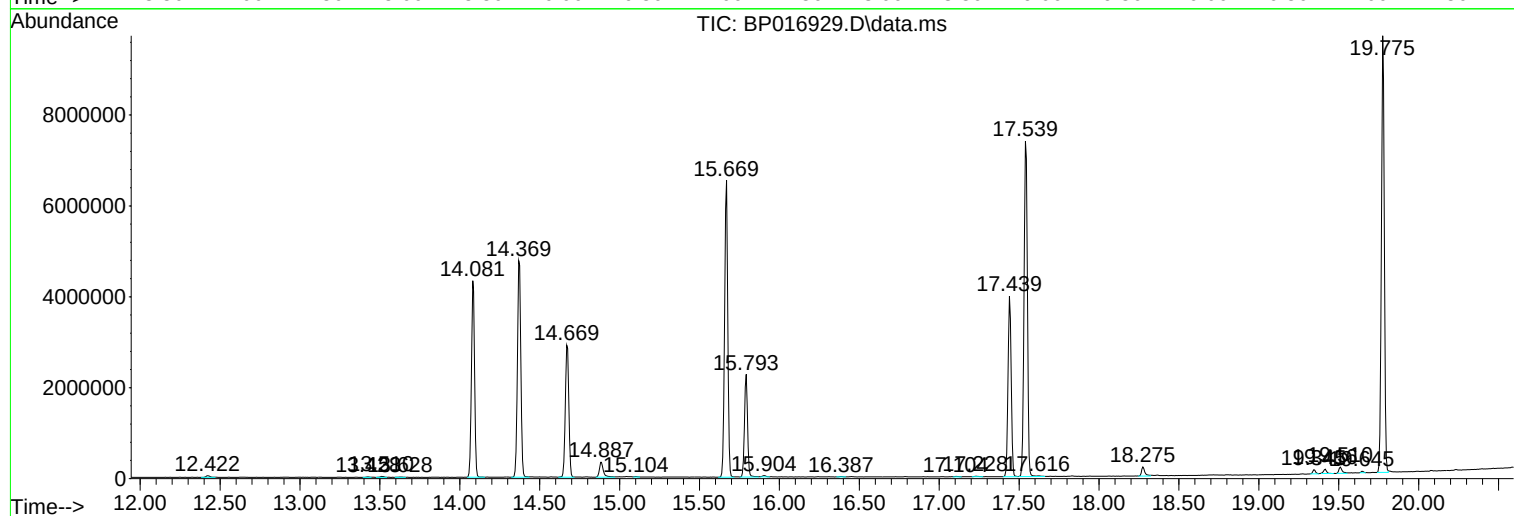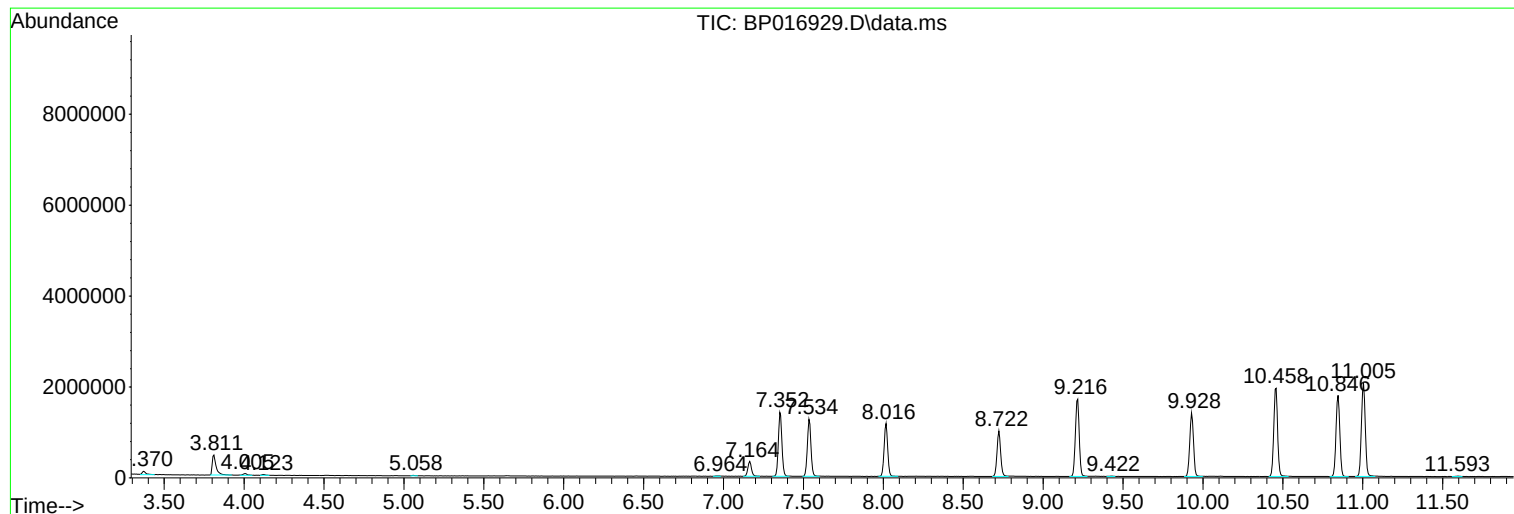

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016929.D
Acq On : 02 Sep 2023 03:48
Operator : MA/JU
Sample : 04209-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH467

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016929.D
Acq On : 02 Sep 2023 03:48
Operator : MA/JU
Sample : 04209-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH467

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc