

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
 Data File : BP016931.D
 Acq On : 02 Sep 2023 04:55
 Operator : MA/JU
 Sample : 04209-06
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH470

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016931.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	11	14	28	rVB	74283	120388	0.86%	0.106%
2	3.811	86	89	103	rBV	233421	379822	2.73%	0.334%
3	4.005	117	122	128	rVB2	40193	65921	0.47%	0.058%
4	4.122	138	142	148	rVB	18107	27876	0.20%	0.024%
5	5.058	298	301	306	rVB2	9939	14555	0.10%	0.013%
6	7.163	652	659	672	rBV	354710	575680	4.14%	0.506%
7	7.352	682	691	701	rBV	1579033	2479736	17.81%	2.178%
8	7.534	715	722	733	rBV	1421809	2234316	16.05%	1.963%
9	8.016	797	804	815	rVB	1062144	1666720	11.97%	1.464%
10	8.722	916	924	942	rBV	1128112	1827450	13.13%	1.605%
11	9.210	1000	1007	1025	rBV	1871878	3169309	22.77%	2.784%
12	9.928	1121	1129	1141	rBV	1585618	2565778	18.43%	2.254%
13	10.452	1210	1218	1229	rBV	2157152	3650297	26.22%	3.206%
14	10.846	1277	1285	1292	rBV	1640993	2721844	19.55%	2.391%
15	11.004	1301	1312	1324	rBV	1921221	3314355	23.81%	2.911%
16	11.593	1406	1412	1424	rBV	10915	31080	0.22%	0.027%
17	12.422	1546	1553	1559	rBV	42795	72144	0.52%	0.063%
18	13.345	1704	1710	1715	rBV3	10352	14423	0.10%	0.013%
19	13.422	1715	1723	1727	rBV4	10672	16767	0.12%	0.015%
20	13.516	1732	1739	1745	rBV	50922	86359	0.62%	0.076%
21	13.628	1755	1758	1764	rVB4	8939	14299	0.10%	0.013%
22	14.081	1828	1835	1848	rBV	4984308	6732141	48.36%	5.913%
23	14.369	1877	1884	1892	rBV2	5518143	7909100	56.82%	6.947%
24	14.440	1893	1896	1903	rVB2	22033	37859	0.27%	0.033%
25	14.669	1929	1935	1947	rVV	2819097	4057070	29.14%	3.564%
26	14.881	1965	1971	1985	rBV	392070	655808	4.71%	0.576%
27	15.098	2005	2008	2014	rVB4	16831	24117	0.17%	0.021%
28	15.669	2095	2105	2113	rBV	6935328	10172920	73.08%	8.935%
29	15.792	2120	2126	2140	rBV	2477170	3417321	24.55%	3.002%
30	15.904	2140	2145	2151	rVB2	32682	51346	0.37%	0.045%
31	17.104	2344	2349	2356	rBV9	10653	23062	0.17%	0.020%
32	17.245	2366	2373	2377	rBV5	11717	24303	0.17%	0.021%
33	17.439	2399	2406	2416	rBV	3722843	5133284	36.88%	4.509%
34	17.539	2416	2423	2438	rVV2	8319730	11955069	85.88%	10.501%
35	18.063	2508	2512	2516	rBV6	9423	16657	0.12%	0.015%
36	18.275	2543	2548	2559	rBV	194070	302801	2.18%	0.266%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
 Data File : BP016931.D
 Acq On : 02 Sep 2023 04:55
 Operator : MA/JU
 Sample : 04209-06
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH470

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

37	19.116	2687	2691	2701	rVB6	36177	64545	0.46%	0.057%
38	19.222	2705	2709	2714	rVV	98477	112914	0.81%	0.099%
39	19.345	2726	2730	2734	rBV	104889	134718	0.97%	0.118%
40	19.410	2737	2741	2746	rVV	96566	137629	0.99%	0.121%
41	19.510	2754	2758	2763	rBV2	96429	137984	0.99%	0.121%
42	19.645	2779	2781	2787	rVB4	27339	32348	0.23%	0.028%
43	19.775	2797	2803	2809	rBV	10652768	13920343	100.00%	12.227%
44	21.198	3042	3045	3055	rVB	159706	237202	1.70%	0.208%
45	21.539	3097	3103	3108	rBV	4188388	5380744	38.65%	4.726%
46	21.598	3110	3113	3116	rVV	137962	160019	1.15%	0.141%
47	23.933	3503	3510	3522	rVB2	6150399	12850571	92.32%	11.287%
48	24.104	3532	3539	3552	rVB	2428384	5118543	36.77%	4.496%




Sum of corrected areas: 113849537

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016931.D
Acq On : 02 Sep 2023 04:55
Operator : MA/JU
Sample : 04209-06
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH470

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

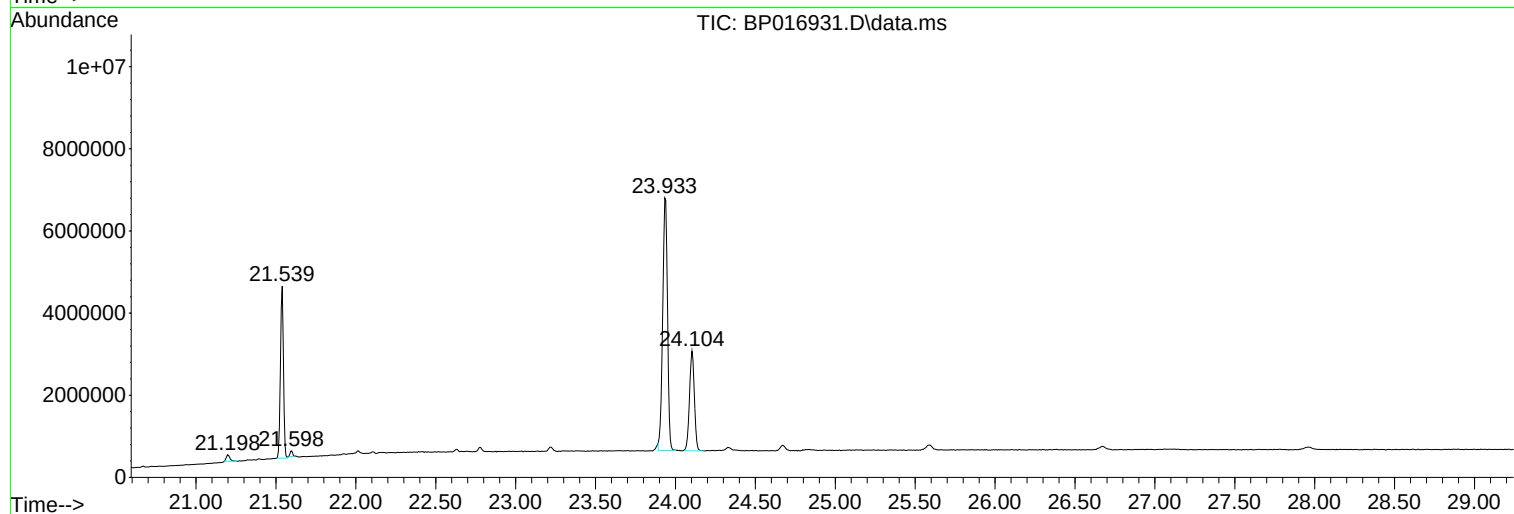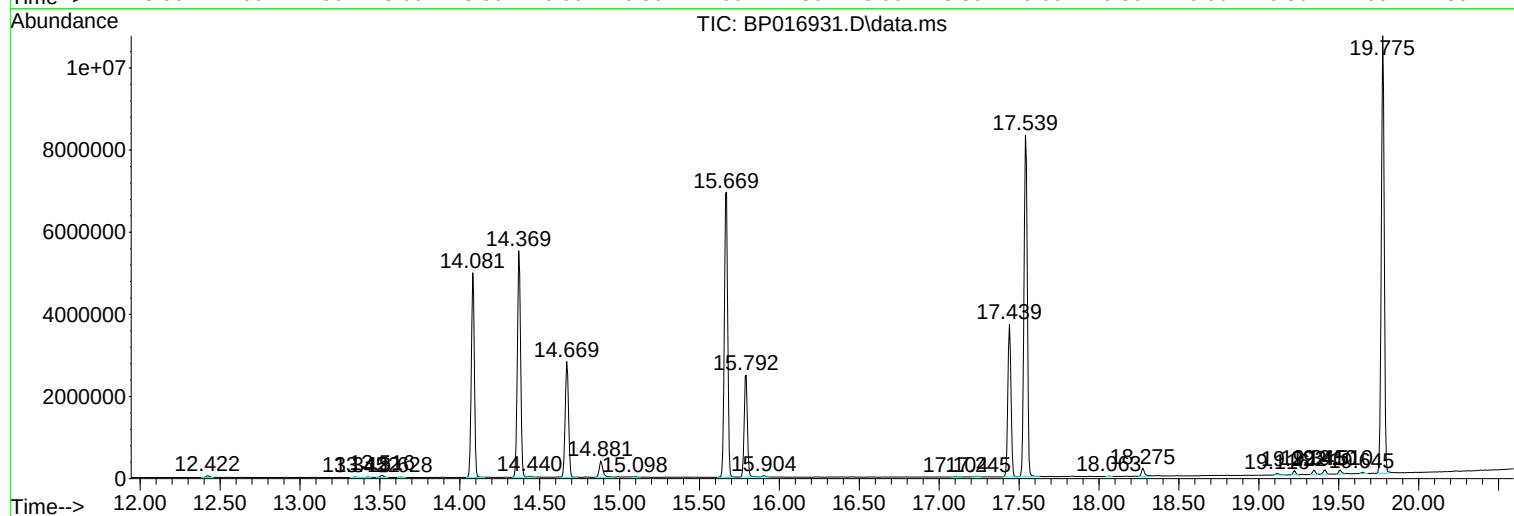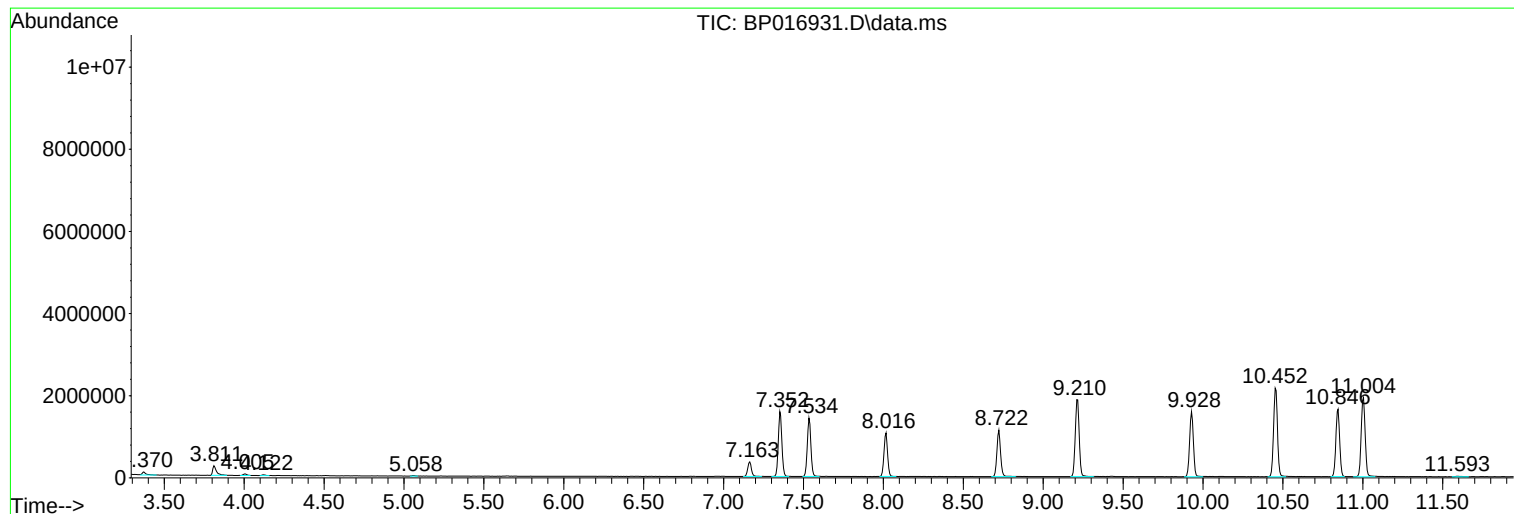

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016931.D
Acq On : 02 Sep 2023 04:55
Operator : MA/JU
Sample : 04209-06
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH470

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016931.D
Acq On : 02 Sep 2023 04:55
Operator : MA/JU
Sample : 04209-06
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH470

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc