

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
 Data File : BP016932.D
 Acq On : 02 Sep 2023 05:29
 Operator : MA/JU
 Sample : 04209-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH482

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016932.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	10	14	29	rVB	81941	139115	1.00%	0.121%
2	3.811	85	89	104	rBV	320242	528763	3.79%	0.458%
3	4.005	117	122	129	rVB	49564	79152	0.57%	0.069%
4	4.117	138	141	151	rVB2	20134	35269	0.25%	0.031%
5	5.058	297	301	307	rVB2	15187	21067	0.15%	0.018%
6	6.958	620	624	633	rBV5	11578	26185	0.19%	0.023%
7	7.163	651	659	671	rBV	450543	716143	5.14%	0.620%
8	7.352	684	691	700	rBV	1661141	2557430	18.34%	2.215%
9	7.534	715	722	738	rVB	1562776	2449748	17.57%	2.122%
10	8.016	797	804	813	rBV	1120979	1755863	12.59%	1.521%
11	8.722	917	924	932	rBV	1325292	2108583	15.12%	1.827%
12	9.210	999	1007	1020	rBV	1989805	3313799	23.77%	2.871%
13	9.928	1120	1129	1142	rBV	1656625	2709023	19.43%	2.347%
14	10.451	1210	1218	1232	rBV	2334680	3906983	28.02%	3.384%
15	10.846	1276	1285	1294	rBV	1725088	2859309	20.51%	2.477%
16	11.004	1304	1312	1329	rBV	2248211	3793463	27.21%	3.286%
17	12.422	1546	1553	1559	rBV2	42449	68348	0.49%	0.059%
18	13.510	1731	1738	1745	rVB	17378	28025	0.20%	0.024%
19	14.081	1827	1835	1842	rBV	5070229	6899568	49.49%	5.977%
20	14.369	1877	1884	1905	rBV2	5602703	8188656	58.74%	7.093%
21	14.669	1925	1935	1944	rBV	2894379	4207165	30.18%	3.644%
22	14.881	1965	1971	1986	rBV	483218	786997	5.65%	0.682%
23	15.098	2005	2008	2016	rVB7	14628	23134	0.17%	0.020%
24	15.669	2097	2105	2111	rBV	7110858	10375005	74.42%	8.987%
25	15.792	2119	2126	2141	rBV	2473202	3426459	24.58%	2.968%
26	15.904	2141	2145	2153	rVB2	32436	50691	0.36%	0.044%
27	17.110	2345	2350	2354	rVB7	9365	16411	0.12%	0.014%
28	17.439	2399	2406	2414	rBV	3745444	5175688	37.13%	4.483%
29	17.539	2416	2423	2434	rBV2	8445887	11976640	85.91%	10.375%
30	17.692	2446	2449	2454	rVB2	9066	15836	0.11%	0.014%
31	18.275	2543	2548	2557	rBV	95746	147132	1.06%	0.127%
32	19.345	2726	2730	2735	rBV	105651	136925	0.98%	0.119%
33	19.410	2737	2741	2750	rVB	100187	145425	1.04%	0.126%
34	19.504	2754	2757	2764	rBV2	89294	131591	0.94%	0.114%
35	19.645	2779	2781	2785	rVB3	25088	24099	0.17%	0.021%
36	19.775	2797	2803	2809	rBV	10858095	13941197	100.00%	12.077%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016932.D
Acq On : 02 Sep 2023 05:29
Operator : MA/JU
Sample : 04209-08
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH482

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Title : SVOA CALIBRATION

37	21.539	3097	3103	3110	rBV	3988732	5412885	38.83%	4.689%
38	23.933	3502	3510	3523	rVB2	6032651	12364085	88.69%	10.710%
39	24.104	3532	3539	3549	rVB	2296060	4897740	35.13%	4.243%




Sum of corrected areas: 115439597

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016932.D
Acq On : 02 Sep 2023 05:29
Operator : MA/JU
Sample : 04209-08
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH482

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

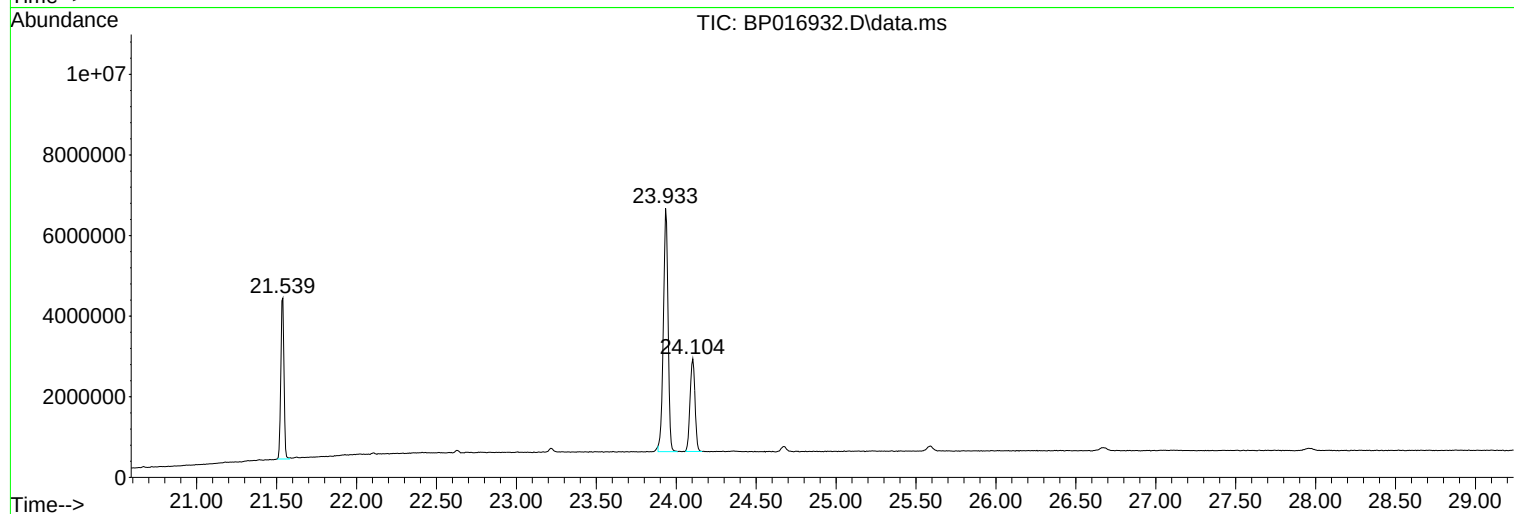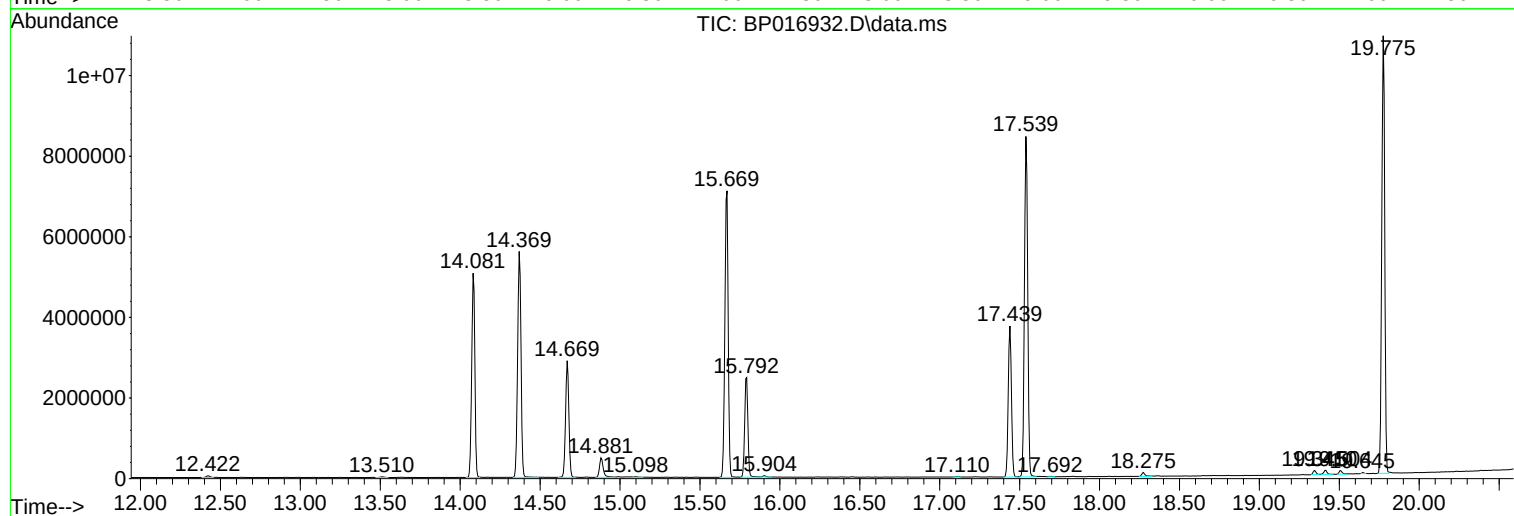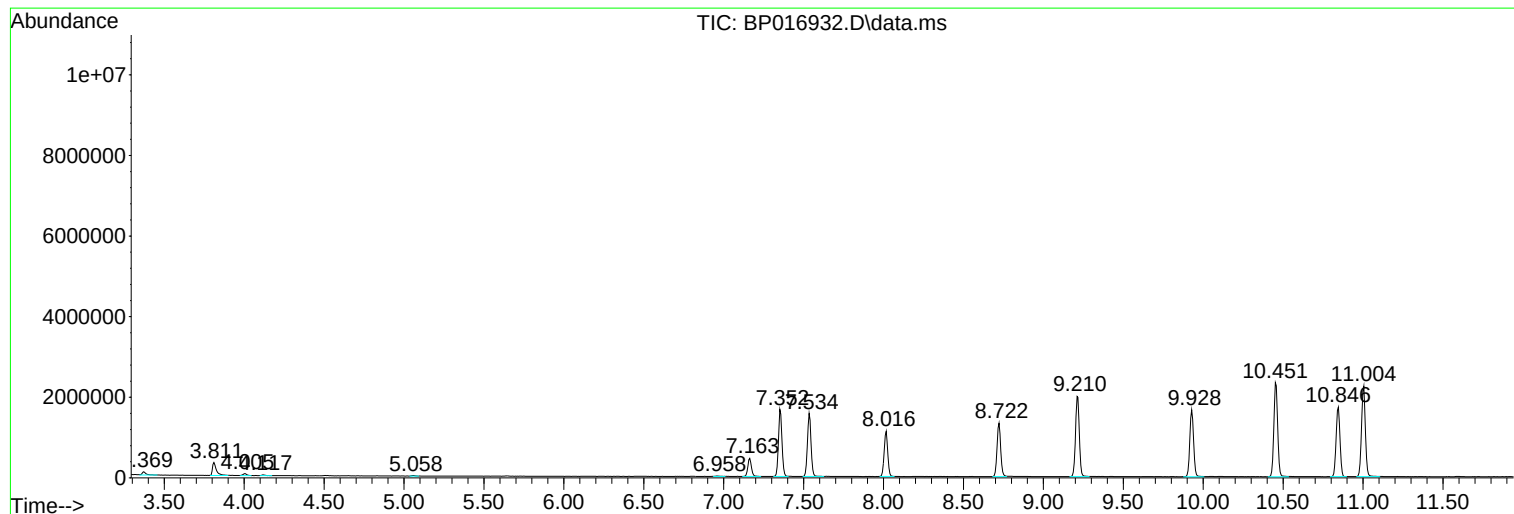

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016932.D
Acq On : 02 Sep 2023 05:29
Operator : MA/JU
Sample : 04209-08
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH482

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016932.D
Acq On : 02 Sep 2023 05:29
Operator : MA/JU
Sample : 04209-08
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH482

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc