

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
 Data File : BP016934.D
 Acq On : 02 Sep 2023 06:36
 Operator : MA/JU
 Sample : 04209-12
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH486

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016934.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	11	14	23	rVB	70611	103808	0.86%	0.105%
2	3.811	85	89	103	rBV	369973	613990	5.10%	0.618%
3	4.005	118	122	129	rVB	35953	54537	0.45%	0.055%
4	4.122	139	142	146	rVB	16029	20343	0.17%	0.020%
5	4.646	227	231	235	rBV6	9967	14782	0.12%	0.015%
6	5.058	297	301	306	rVB	12285	20591	0.17%	0.021%
7	7.163	653	659	667	rBV	315833	501870	4.17%	0.505%
8	7.352	684	691	703	rBV	1269707	1951103	16.20%	1.964%
9	7.534	715	722	736	rVB	1147250	1797315	14.92%	1.809%
10	8.016	796	804	815	rBV	1095006	1722050	14.30%	1.734%
11	8.722	917	924	935	rBV	944545	1535198	12.75%	1.545%
12	9.210	998	1007	1020	rBV	1512386	2497146	20.73%	2.514%
13	9.928	1119	1129	1141	rBV	1283685	2046844	16.99%	2.061%
14	10.451	1210	1218	1228	rBV	1744990	2906410	24.13%	2.926%
15	10.840	1277	1284	1292	rBV	1643478	2776509	23.05%	2.795%
16	11.004	1303	1312	1330	rBV	1806957	3086268	25.62%	3.107%
17	12.422	1547	1553	1561	rBV2	31380	53773	0.45%	0.054%
18	13.516	1732	1739	1745	rBV	43390	72360	0.60%	0.073%
19	14.081	1827	1835	1844	rBV	4145488	5368968	44.58%	5.405%
20	14.369	1876	1884	1894	rBV	4350730	6255135	51.93%	6.297%
21	14.669	1926	1935	1943	rVB	2836409	4077928	33.86%	4.105%
22	14.881	1965	1971	1984	rBV	362047	594925	4.94%	0.599%
23	14.992	1986	1990	1994	rVB3	9805	15833	0.13%	0.016%
24	15.098	2004	2008	2015	rVB6	16750	28803	0.24%	0.029%
25	15.663	2097	2104	2112	rBV	5778041	8358335	69.40%	8.414%
26	15.786	2119	2125	2139	rBV	2182881	2964654	24.61%	2.984%
27	15.904	2140	2145	2154	rVB2	28134	47159	0.39%	0.047%
28	16.398	2224	2229	2234	rVB4	11480	20105	0.17%	0.020%
29	17.104	2346	2349	2357	rVB10	8726	15408	0.13%	0.016%
30	17.222	2365	2369	2378	rBV4	9082	16384	0.14%	0.016%
31	17.439	2399	2406	2415	rBV	3649105	5062972	42.04%	5.097%
32	17.539	2416	2423	2433	rBV2	7242926	10357817	86.00%	10.427%
33	18.063	2509	2512	2516	rVB5	12813	14142	0.12%	0.014%
34	18.269	2543	2547	2558	rBV	126243	209240	1.74%	0.211%
35	19.345	2726	2730	2734	rBV2	83351	103670	0.86%	0.104%
36	19.416	2737	2742	2746	rVV	86533	116245	0.97%	0.117%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016934.D
Acq On : 02 Sep 2023 06:36
Operator : MA/JU
Sample : 04209-12
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH486

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Title : SVOA CALIBRATION

37	19.510	2754	2758	2766	rBV2	96452	144932	1.20%	0.146%
38	19.645	2778	2781	2786	rBV2	36833	43567	0.36%	0.044%
39	19.774	2797	2803	2809	rBV	9293782	12044460	100.00%	12.125%
40	21.180	3039	3042	3043	rBV3	67813	77027	0.64%	0.078%
41	21.533	3097	3102	3109	rBV	4076319	5359643	44.50%	5.396%
42	23.933	3502	3510	3523	rVB2	5255856	11231378	93.25%	11.307%
43	24.104	3532	3539	3548	rVB	2386751	5031683	41.78%	5.065%




Sum of corrected areas: 99335310

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016934.D
Acq On : 02 Sep 2023 06:36
Operator : MA/JU
Sample : 04209-12
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH486

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

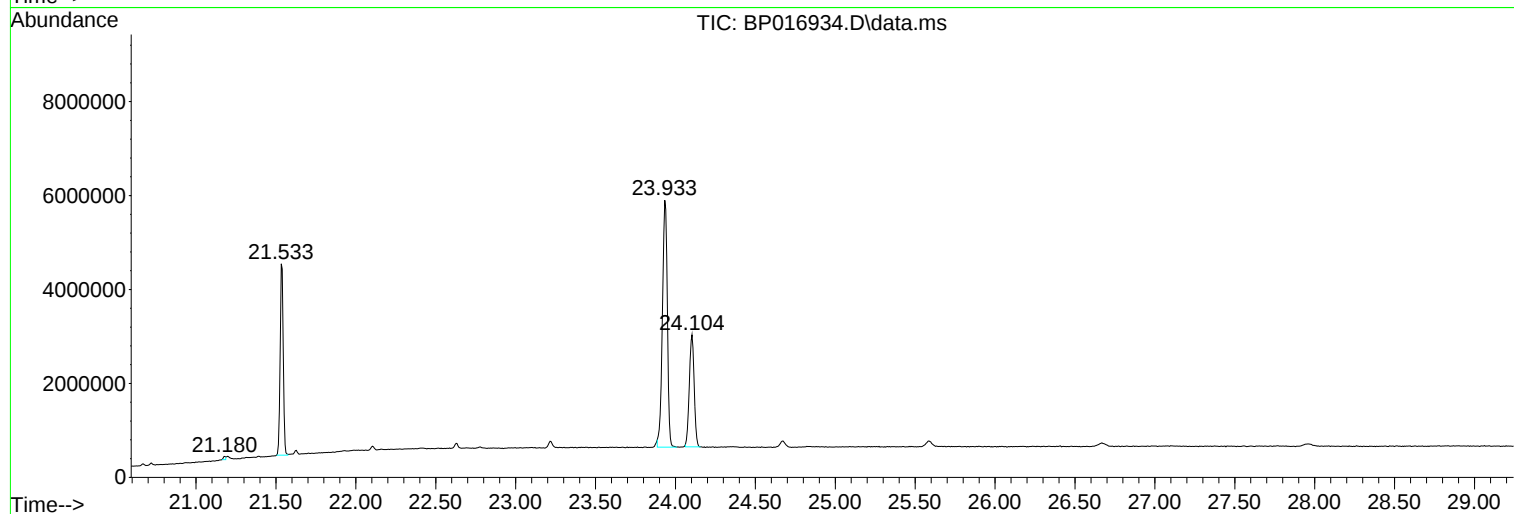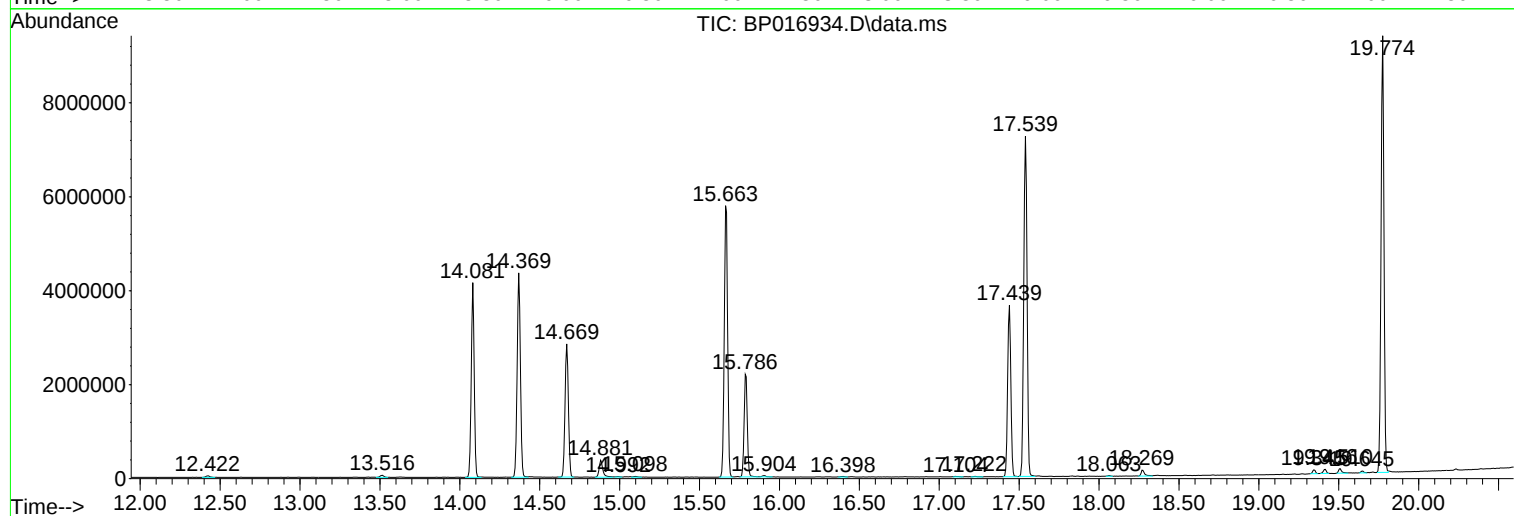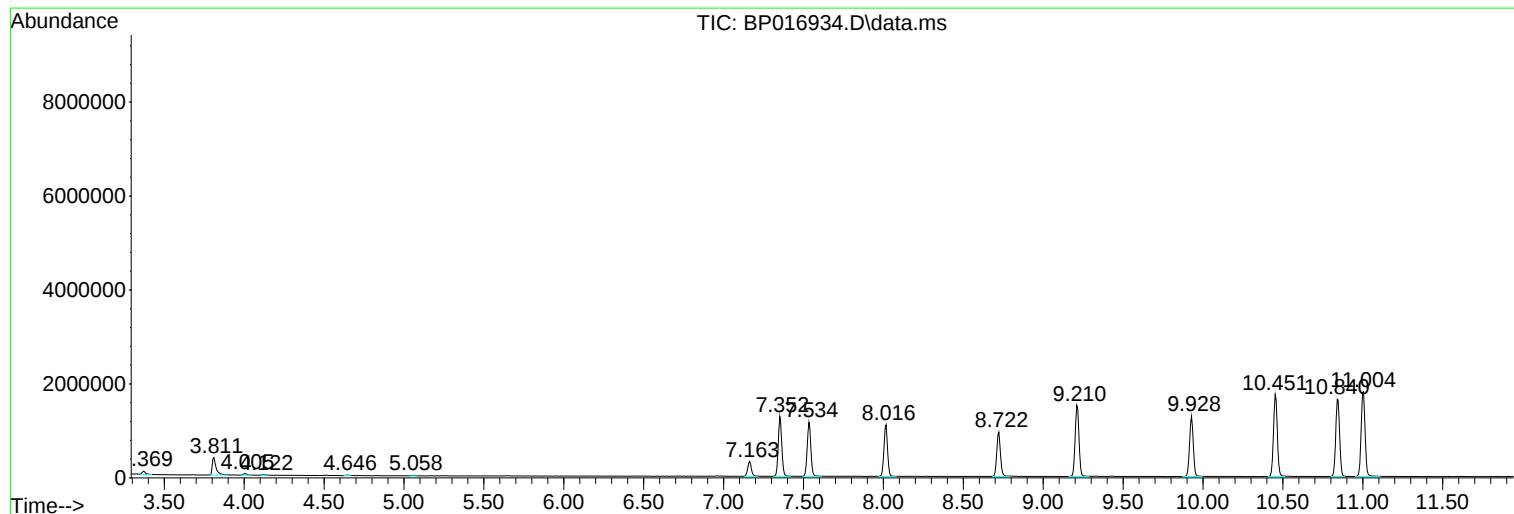

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016934.D
Acq On : 02 Sep 2023 06:36
Operator : MA/JU
Sample : 04209-12
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH486

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016934.D
Acq On : 02 Sep 2023 06:36
Operator : MA/JU
Sample : 04209-12
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH486

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------