

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
 Data File : BP016938.D
 Acq On : 02 Sep 2023 08:50
 Operator : MA/JU
 Sample : 04209-20
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH488

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016938.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.323	3	6	11	rBV	128754	186846	1.04%	0.164%
2	3.370	11	14	25	rVB	69788	118340	0.66%	0.104%
3	3.805	85	88	105	rBV	448221	749617	4.19%	0.656%
4	3.999	118	121	130	rVB	37692	63245	0.35%	0.055%
5	4.646	227	231	238	rVB2	31284	47539	0.27%	0.042%
6	7.164	651	659	670	rBV	338017	552036	3.08%	0.483%
7	7.352	683	691	702	rBV	1401824	2141363	11.96%	1.875%
8	7.534	715	722	736	rBV	1244008	1967170	10.99%	1.722%
9	8.011	796	803	814	rBV	893241	1442427	8.06%	1.263%
10	8.722	916	924	935	rBV	1020929	1658033	9.26%	1.452%
11	9.210	999	1007	1019	rBV	1690606	2716082	15.17%	2.378%
12	9.928	1120	1129	1140	rBV	1346882	2181869	12.19%	1.910%
13	10.452	1210	1218	1229	rBV	1950116	3159810	17.65%	2.766%
14	10.840	1276	1284	1296	rVB	1369173	2324197	12.98%	2.035%
15	10.999	1303	1311	1321	rBV	1912282	3268053	18.26%	2.861%
16	12.357	1535	1542	1547	rBV	27292	44131	0.25%	0.039%
17	12.422	1547	1553	1561	rVB2	33934	57163	0.32%	0.050%
18	13.510	1733	1738	1745	rBV	39082	63794	0.36%	0.056%
19	14.081	1828	1835	1843	rBV	4313180	5627017	31.43%	4.926%
20	14.369	1877	1884	1895	rBV	4664112	6638105	37.08%	5.811%
21	14.669	1924	1935	1944	rBV	2352974	3423779	19.13%	2.997%
22	14.881	1965	1971	1984	rBV	339236	568857	3.18%	0.498%
23	14.993	1986	1990	1994	rVB	29141	37631	0.21%	0.033%
24	15.663	2096	2104	2112	rBV	5872299	8441803	47.16%	7.391%
25	15.787	2119	2125	2140	rBV	2067746	2765197	15.45%	2.421%
26	15.898	2140	2144	2151	rVB2	26629	42671	0.24%	0.037%
27	17.263	2366	2376	2380	rBV	11788242	17901579	100.00%	15.672%
28	17.439	2399	2406	2416	rBV	3067351	4258398	23.79%	3.728%
29	17.539	2416	2423	2434	rBV	6979675	9660772	53.97%	8.458%
30	17.692	2444	2449	2453	rBV	13804	18224	0.10%	0.016%
31	18.275	2543	2548	2556	rBV	97899	153025	0.85%	0.134%
32	18.363	2560	2563	2567	rVB	19652	26081	0.15%	0.023%
33	19.310	2721	2724	2727	rBV2	36376	49689	0.28%	0.044%
34	19.345	2727	2730	2734	rVV2	87266	111726	0.62%	0.098%
35	19.410	2737	2741	2746	rVB	78714	115052	0.64%	0.101%
36	19.510	2754	2758	2763	rBV3	80928	110137	0.62%	0.096%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016938.D
Acq On : 02 Sep 2023 08:50
Operator : MA/JU
Sample : 04209-20
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH488

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Title : SVOA CALIBRATION

37	19.651	2779	2782	2787	rVB5	23662	29328	0.16%	0.026%
38	19.775	2797	2803	2809	rBV	9014776	11551285	64.53%	10.113%
39	21.539	3097	3103	3109	rBV	3471654	4601588	25.70%	4.029%
40	23.933	3502	3510	3520	rVB2	5229319	10896067	60.87%	9.539%
41	24.104	3532	3539	3552	rVB	2095376	4454611	24.88%	3.900%




Sum of corrected areas: 114224337

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016938.D
Acq On : 02 Sep 2023 08:50
Operator : MA/JU
Sample : 04209-20
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH488

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

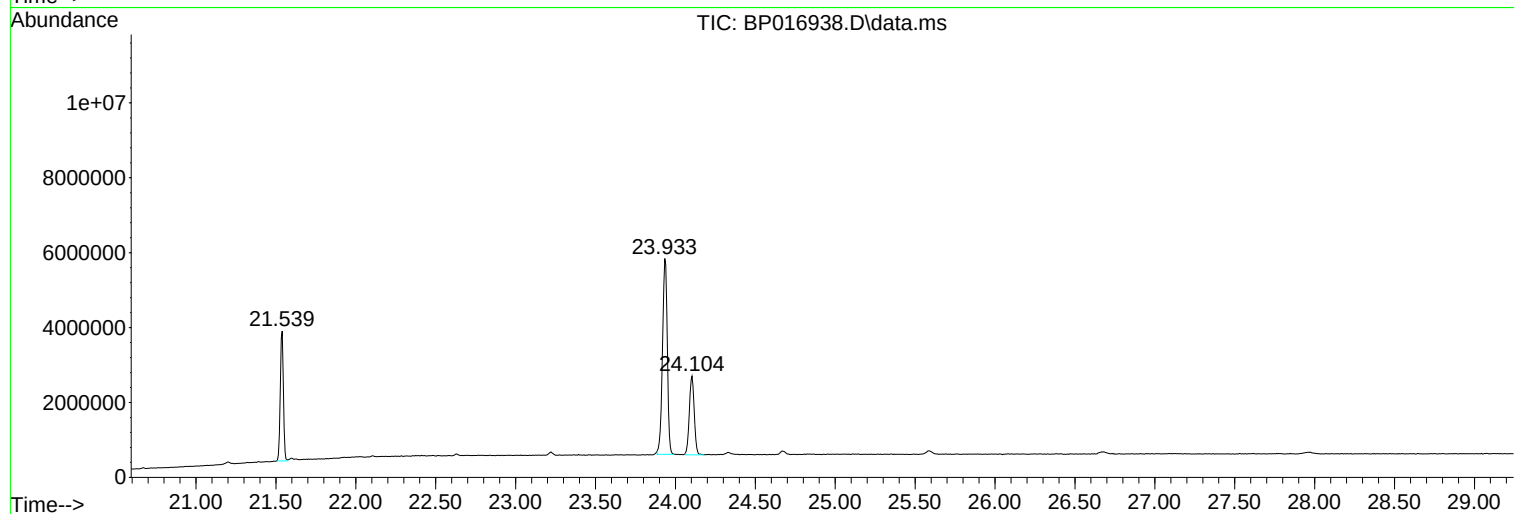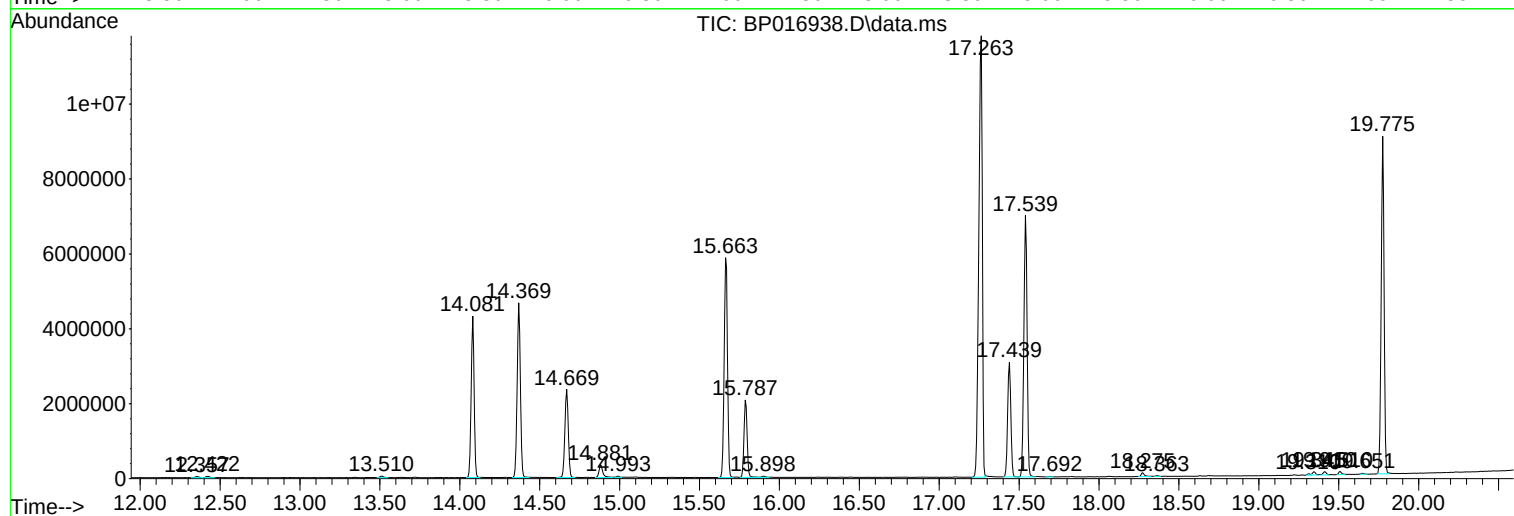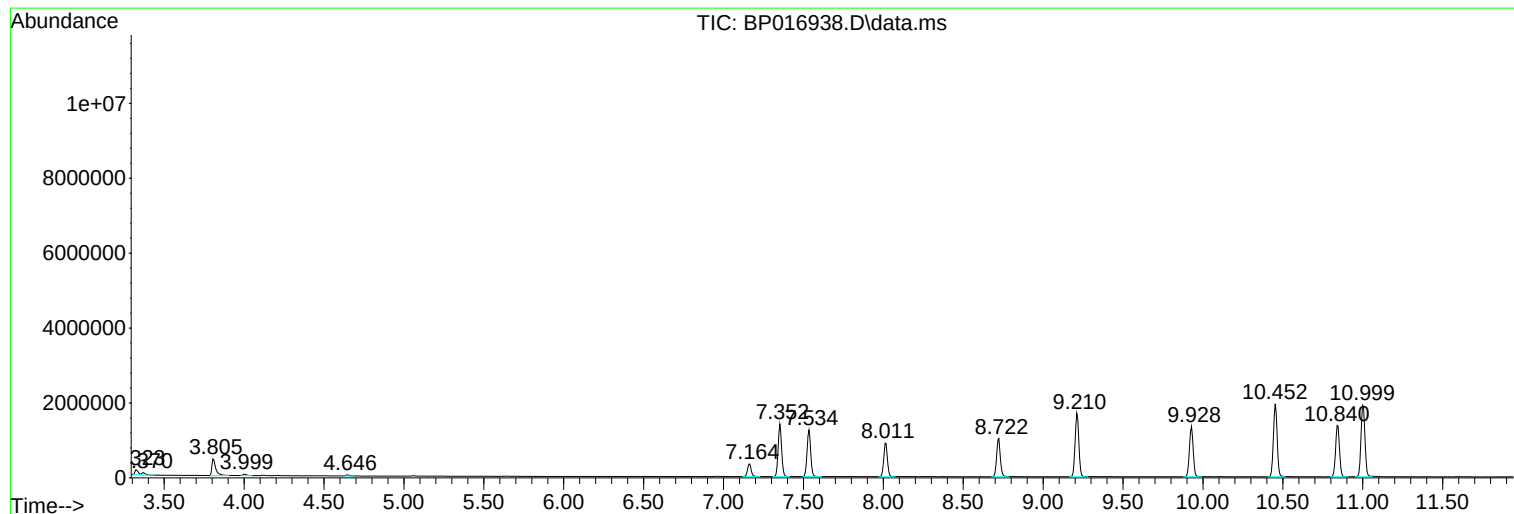

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016938.D
Acq On : 02 Sep 2023 08:50
Operator : MA/JU
Sample : 04209-20
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH488










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzenesulfonamide, N-butyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
17.263	84.08 ng/ul	17901600	Phenanthrene-d10	17.439

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzenesulfonamide, N-butyl-	213	C10H15NO2S	003622-84-2	95
2			Benzenesulfonamide, N-butyl-	213	C10H15NO2S	003622-84-2	90
3			2-propenoic acid, 2-methyl-, 2-[...]	269	C12H15NO4S	1000401-71-8	64
4			Malononitrile, 2-phenylazo-	170	C9H6N4	006017-21-6	50
5			N-hexylbenzenesulfonamide	241	C12H19NO2S	007250-80-8	50

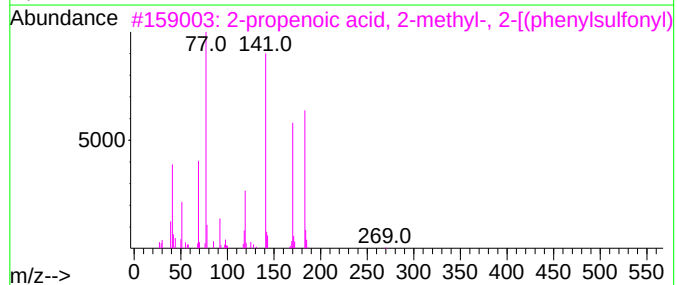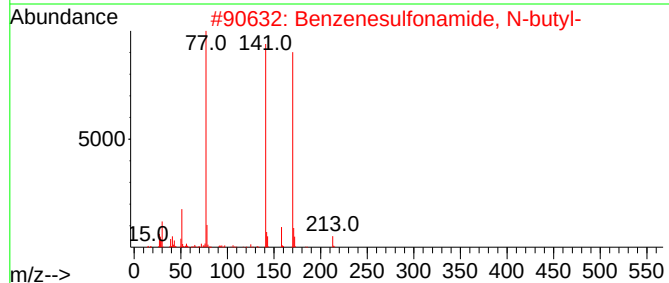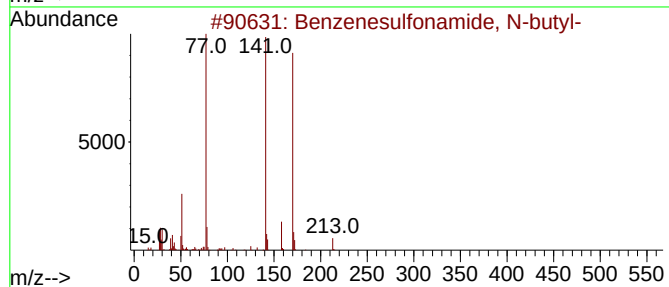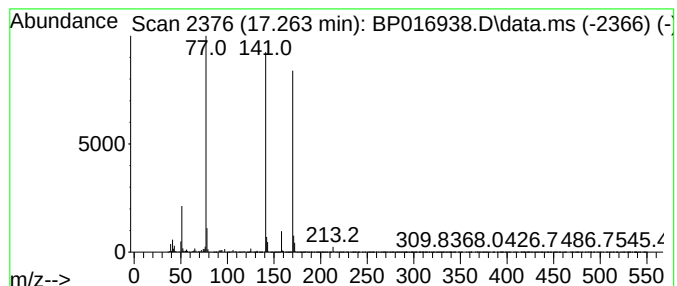

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090123\
Data File : BP016938.D
Acq On : 02 Sep 2023 08:50
Operator : MA/JU
Sample : 04209-20
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH488

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzenesulfonam...	17.263	84.1	ng/ul	17901600	4	17.439	4258400	20.0