
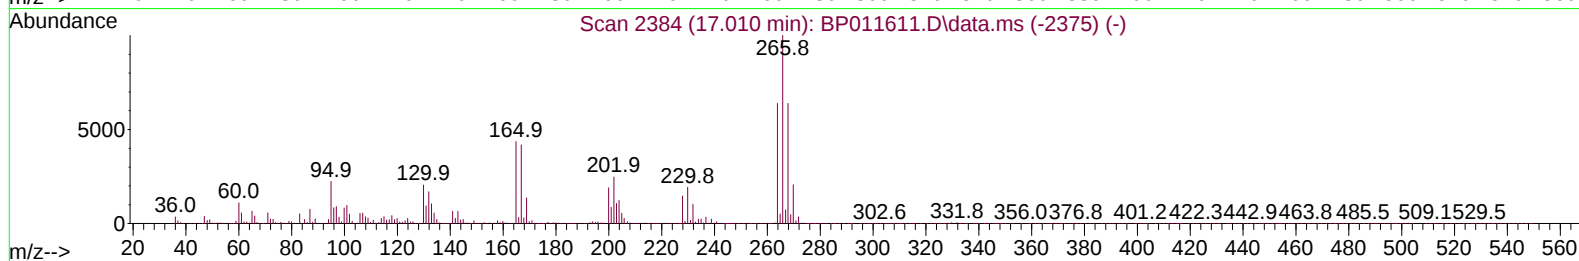
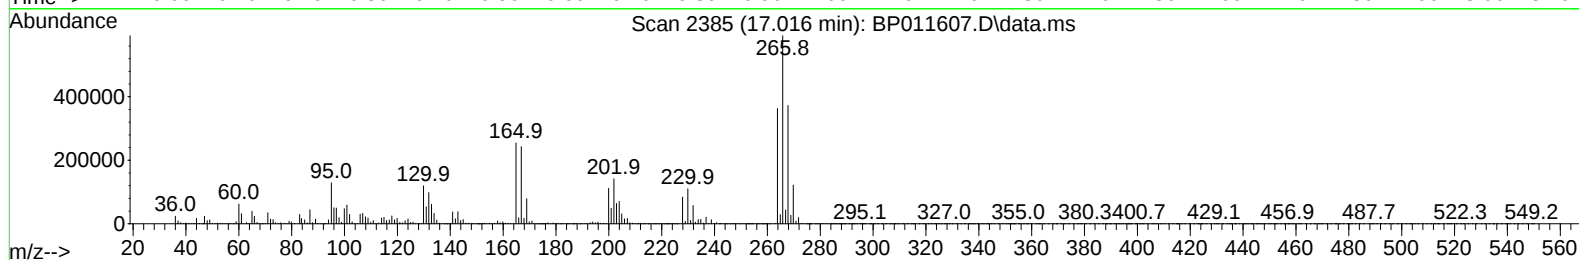


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090222\
Data File : BP011607.D
Acq On : 02 Sep 2022 11:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 02 15:02:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 02 14:35:54 2022
Response via : Initial Calibration

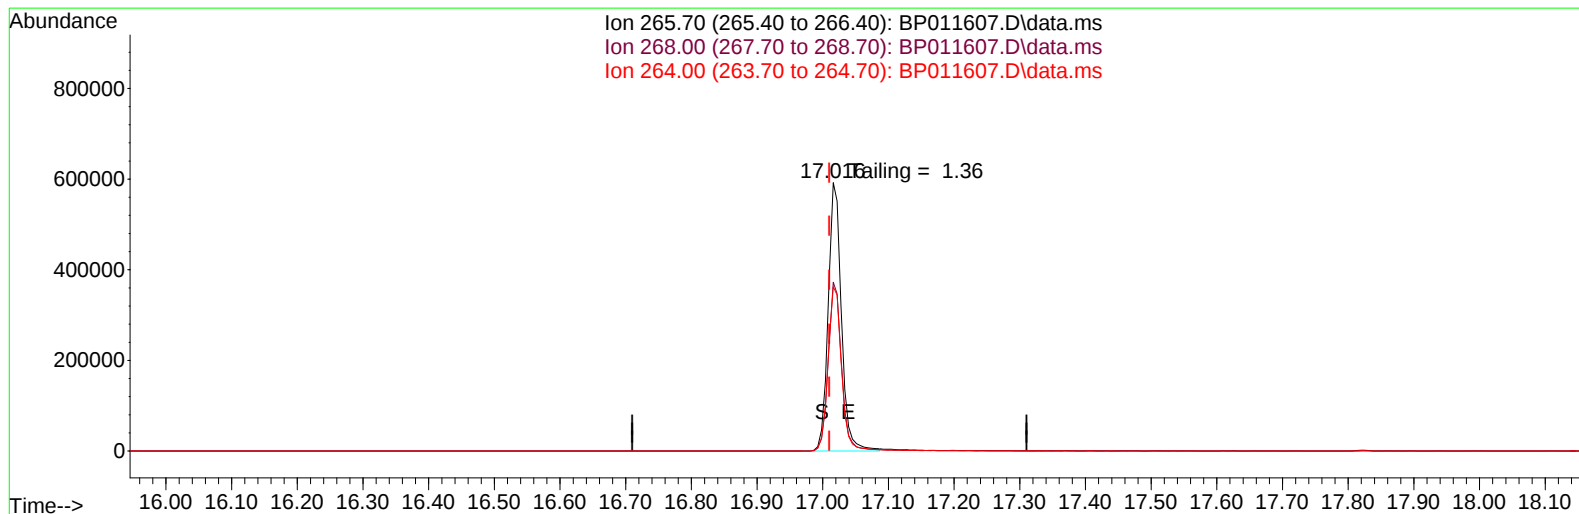

TIC: BP011607.D\data.ms

(70) Pentachlorophenol (C)




17.016min (+ 0.006) 3251529.94 ng

response 836352

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.89
264.00	63.00	61.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090222\
 Data File : BP011607.D
 Acq On : 02 Sep 2022 11:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 02 15:02:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 02 14:35:54 2022
 Response via : Initial Calibration

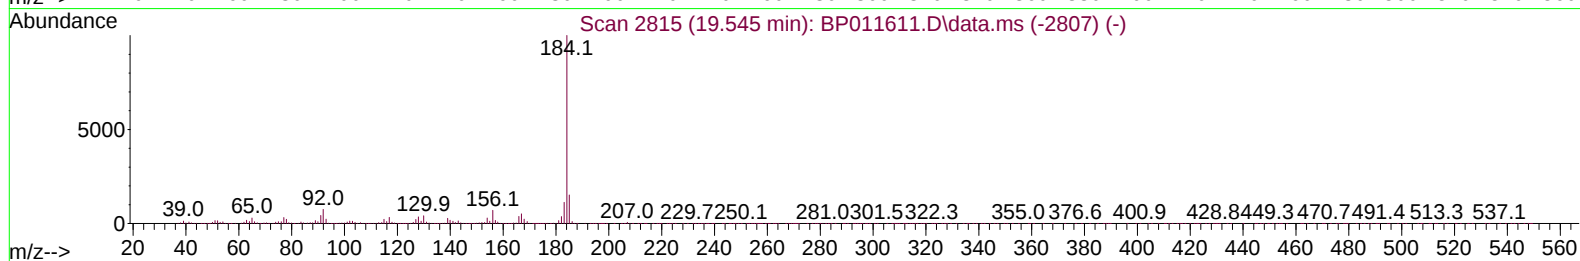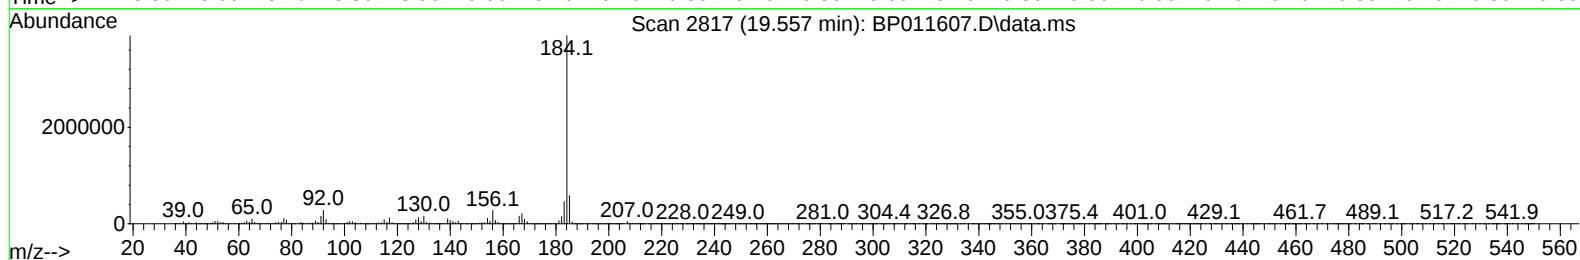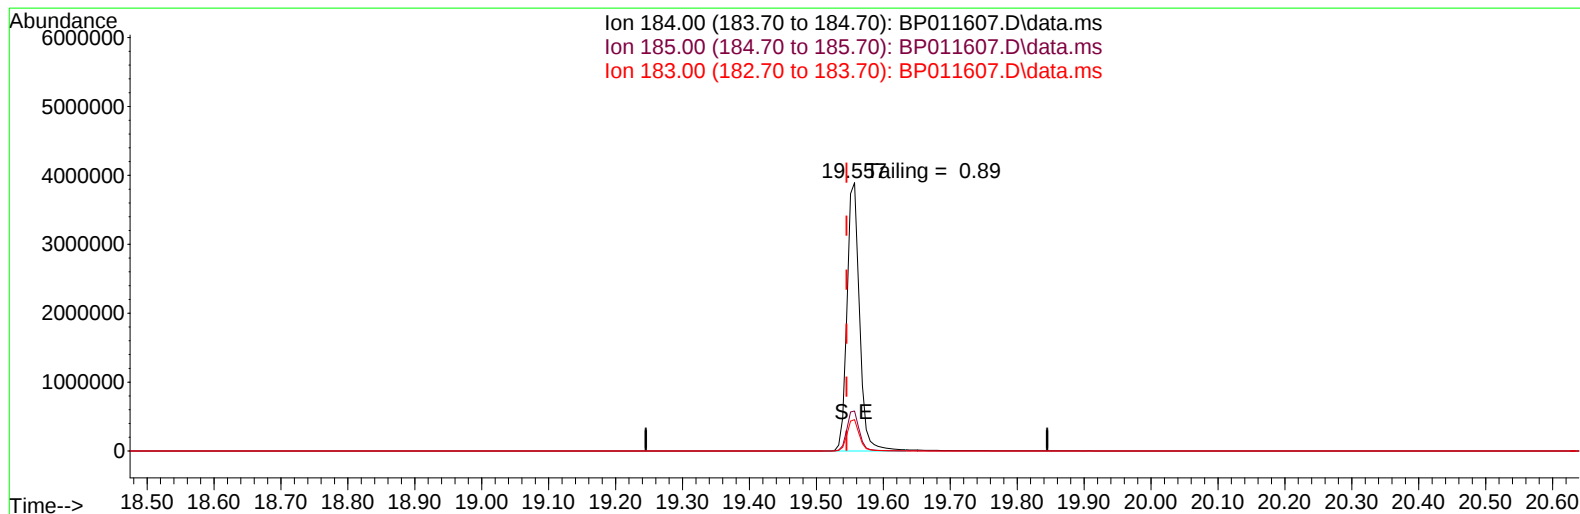

TIC: BP011607.D\data.ms

(77) Benzidine**19.557min (+ 0.012) 1028492.59 ng****response 5065739**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.92
183.00	11.30	11.71
0.00	0.00	0.00