


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090222\
 Data File : BP011607.D
 Acq On : 02 Sep 2022 11:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Sep 03 04:07:09 2022

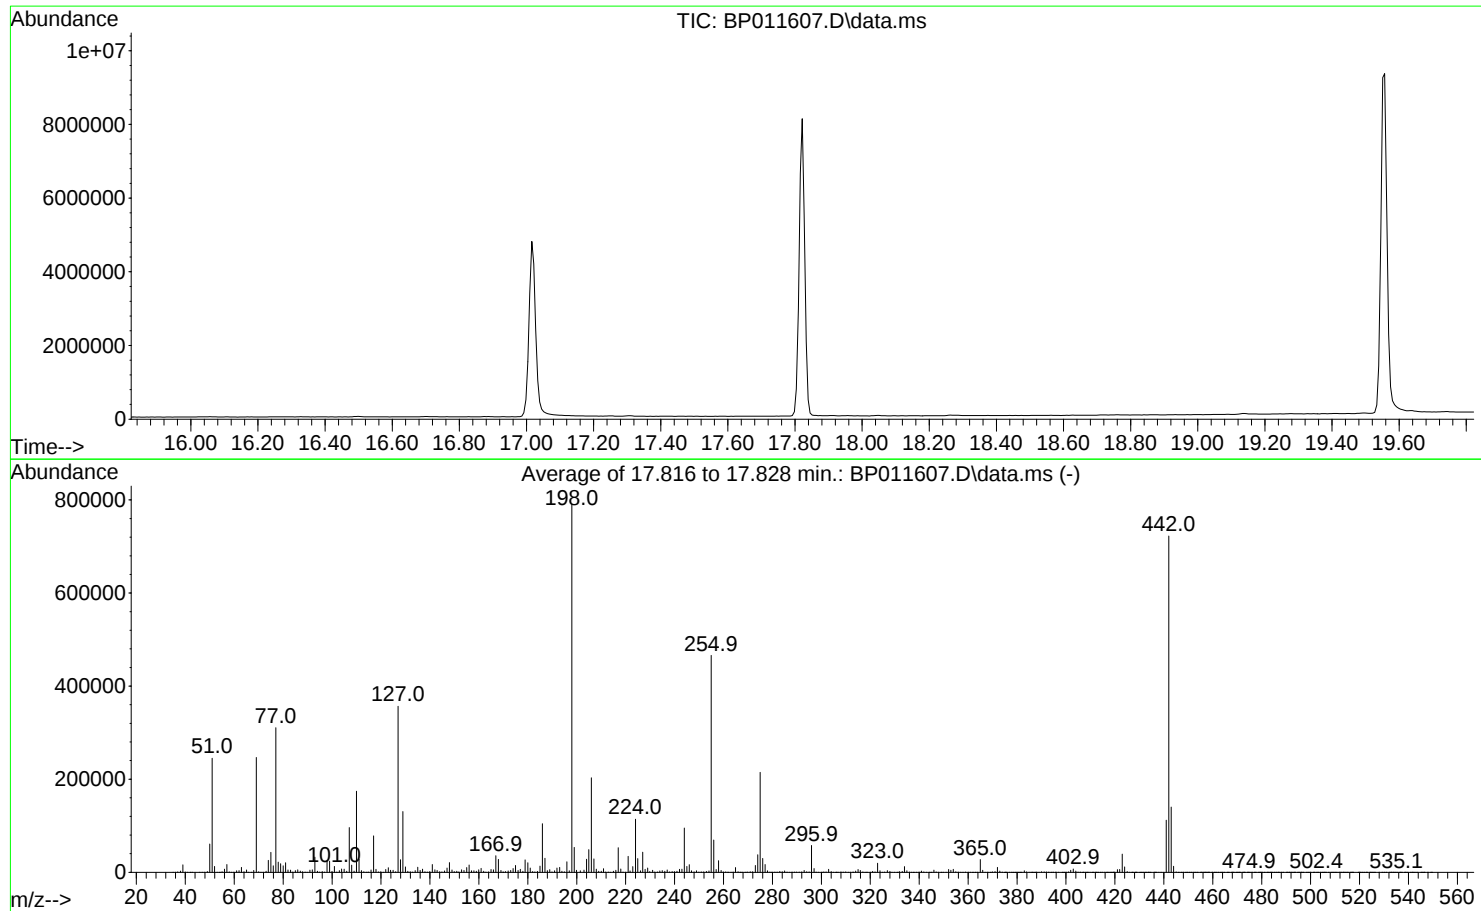


AutoFind: Scans 2521, 2522, 2523; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.0	245016	PASS
68	69	0.00	2	1.6	4056	PASS
69	198	0.00	100	31.2	246702	PASS
70	69	0.00	2	0.5	1298	PASS
127	198	10	80	45.1	356624	PASS
197	198	0.00	2	0.4	3271	PASS
198	198	100	100	100.0	790387	PASS
199	198	5	9	6.8	53659	PASS
275	198	10	60	27.2	214840	PASS
365	198	1	100	3.4	27208	PASS
441	198	0.01	100	14.2	112040	PASS
442	442	100	100	100.0	722509	PASS
443	442	15	24	19.4	139996	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090222\
Data File : BP011607.D
Acq On : 02 Sep 2022 11:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 02 15:02:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 02 14:35:54 2022
Response via : Initial Calibration

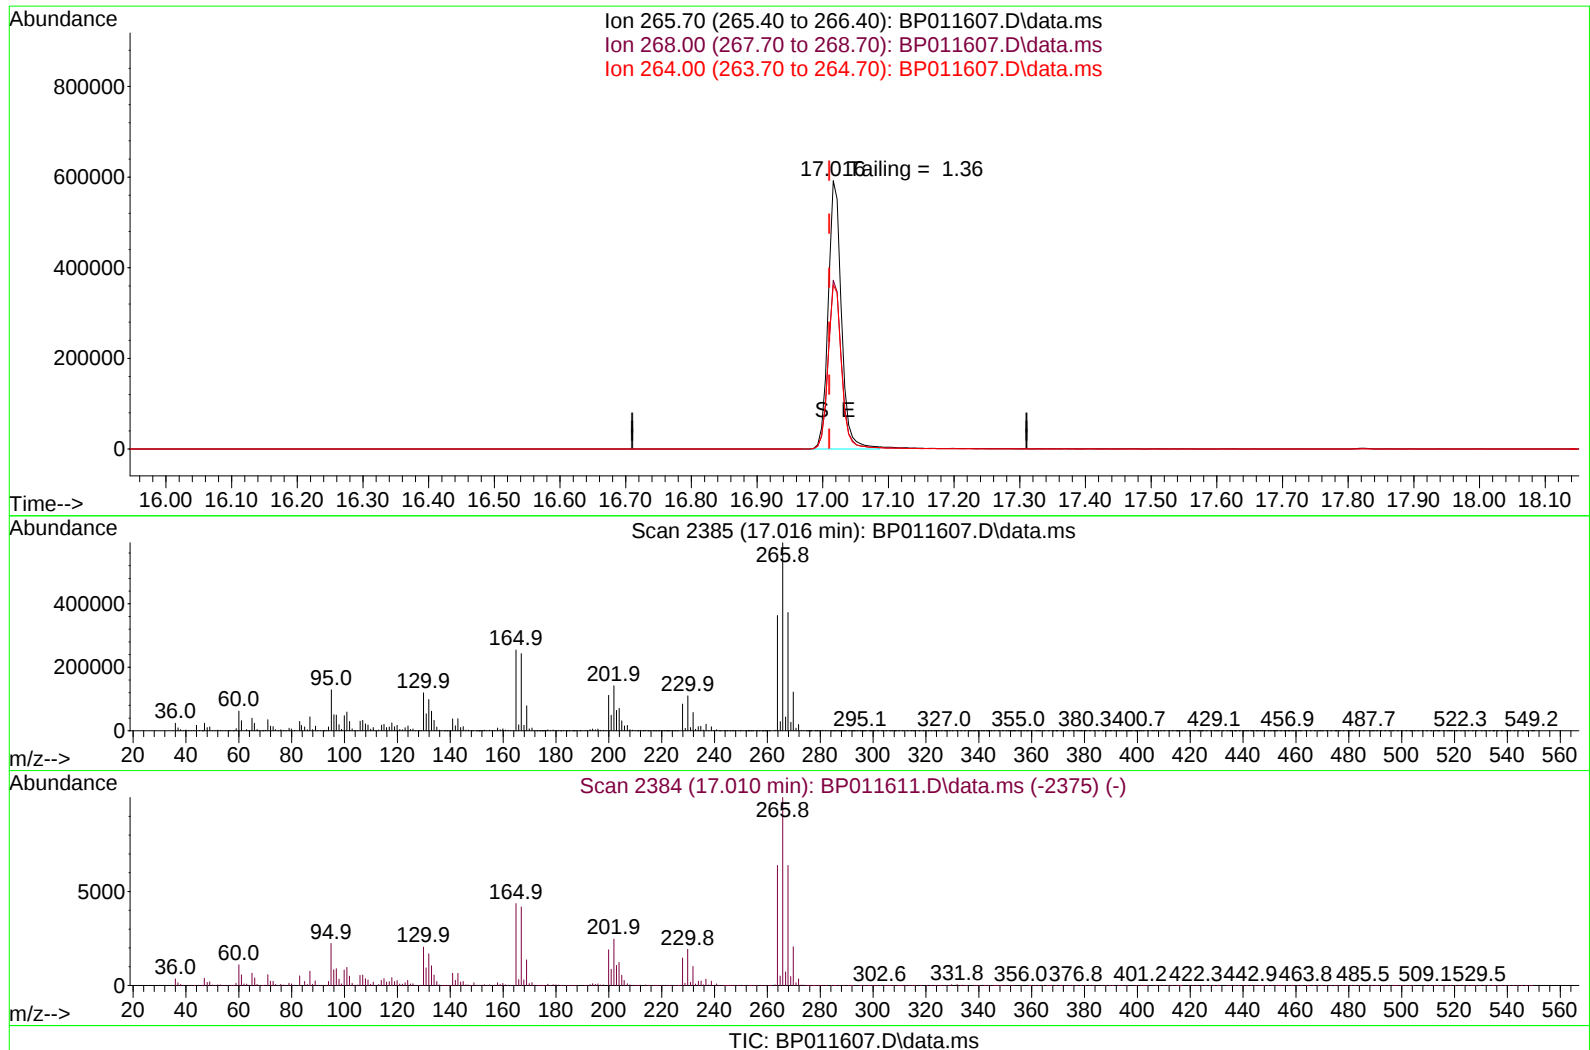

(70) Pentachlorophenol (C)

17.016min (+ 0.006) 3251529.94 ng




response 836352

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.89
264.00	63.00	61.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090222\
 Data File : BP011607.D
 Acq On : 02 Sep 2022 11:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 02 15:02:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 02 14:35:54 2022
 Response via : Initial Calibration

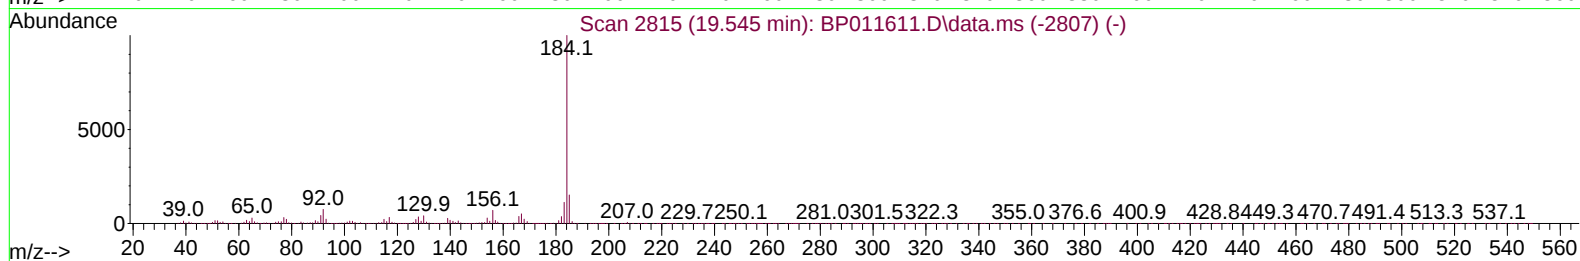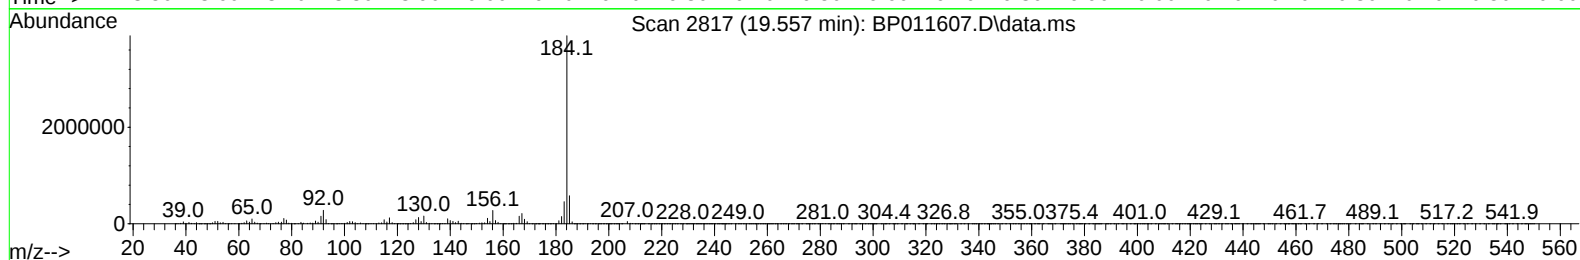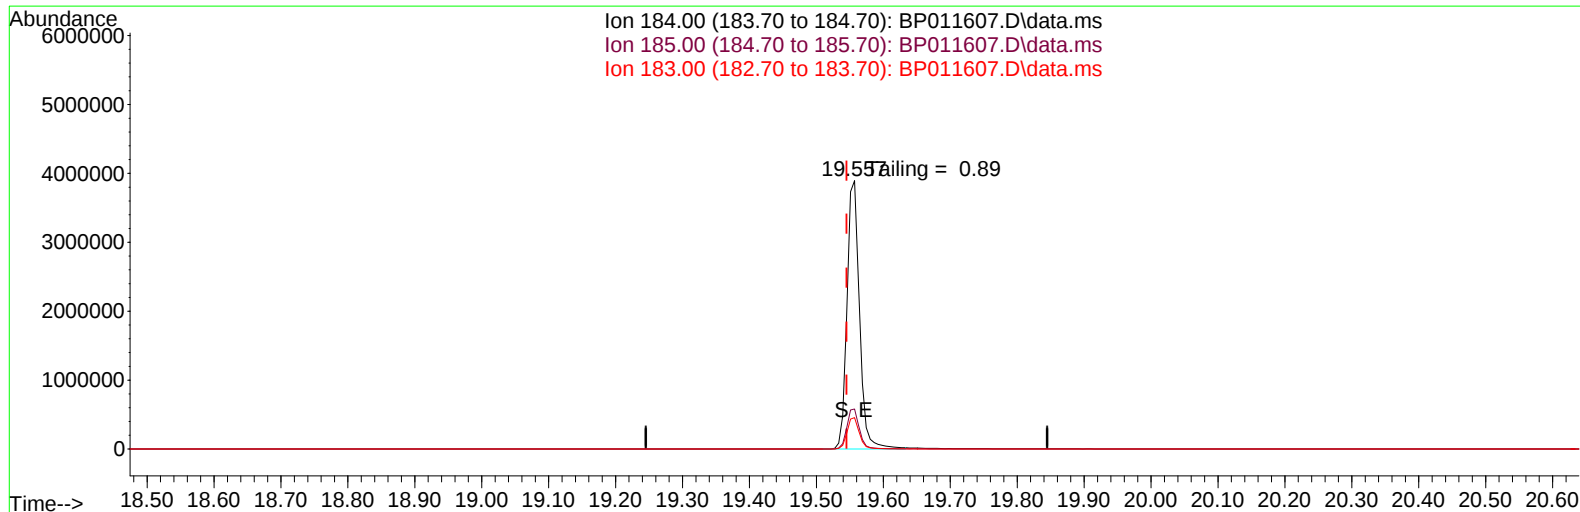

TIC: BP011607.D\data.ms

(77) Benzidine

19.557min (+ 0.012) 1028492.59 ng

response 5065739

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.92
183.00	11.30	11.71
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/2/2022	BNA_P	<u>BP011607.D</u>
Compound Name	Response	Retention Time
DDT	2344118	20.76
DDD	17309	20.32
DDE	686	19.83
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17995	2362113	0.76

Instrument :
BNA_P
ClientSampleId :
DFTPP