
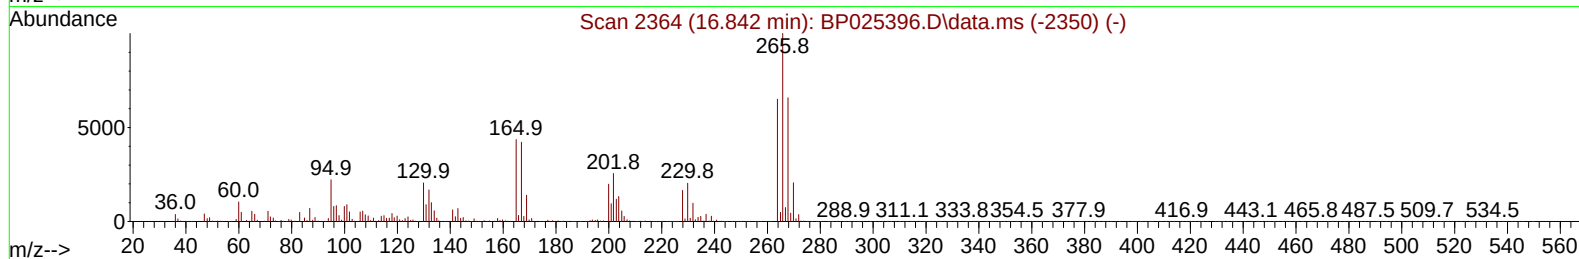
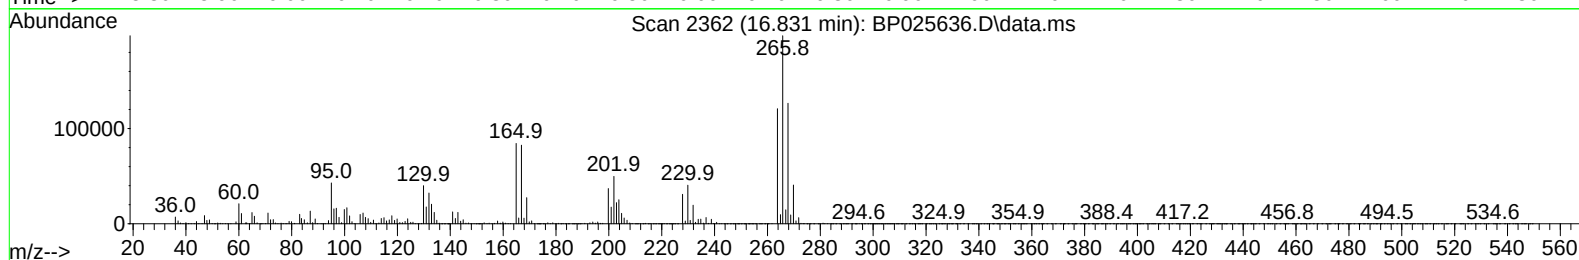


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090225\
Data File : BP025636.D
Acq On : 02 Sep 2025 13:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 02 14:38:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

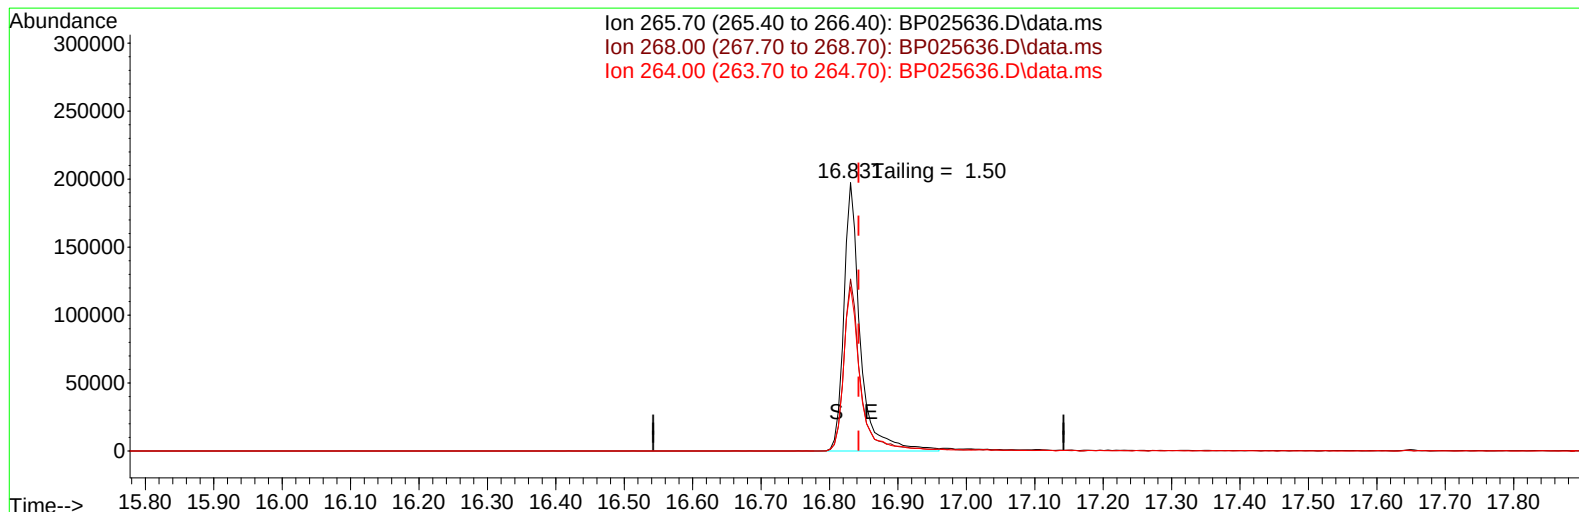

TIC: BP025636.D\data.ms

(70) Pentachlorophenol (C)




16.831min (-0.012) 2157219.78 ng

response 312500

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	64.08
264.00	65.00	61.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090225\
Data File : BP025636.D
Acq On : 02 Sep 2025 13:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 02 14:38:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

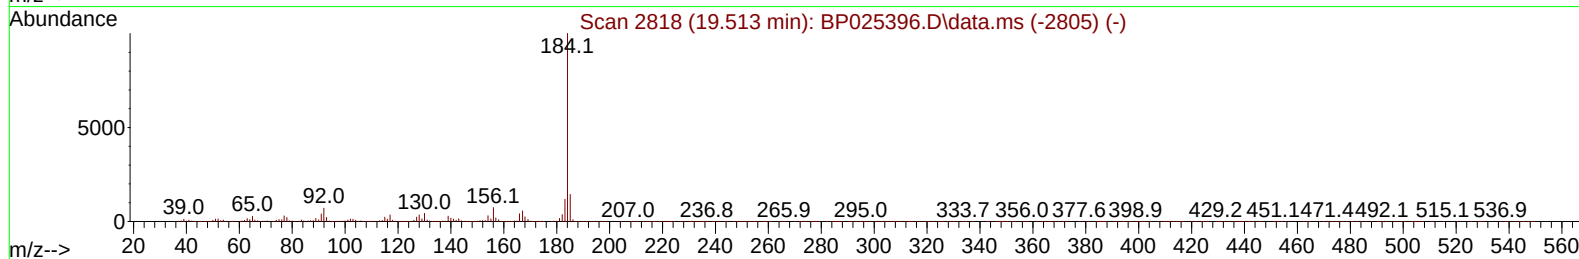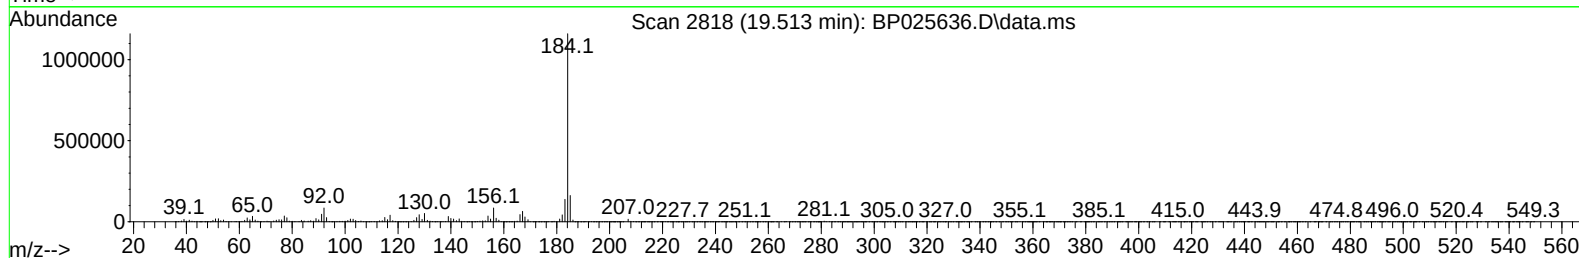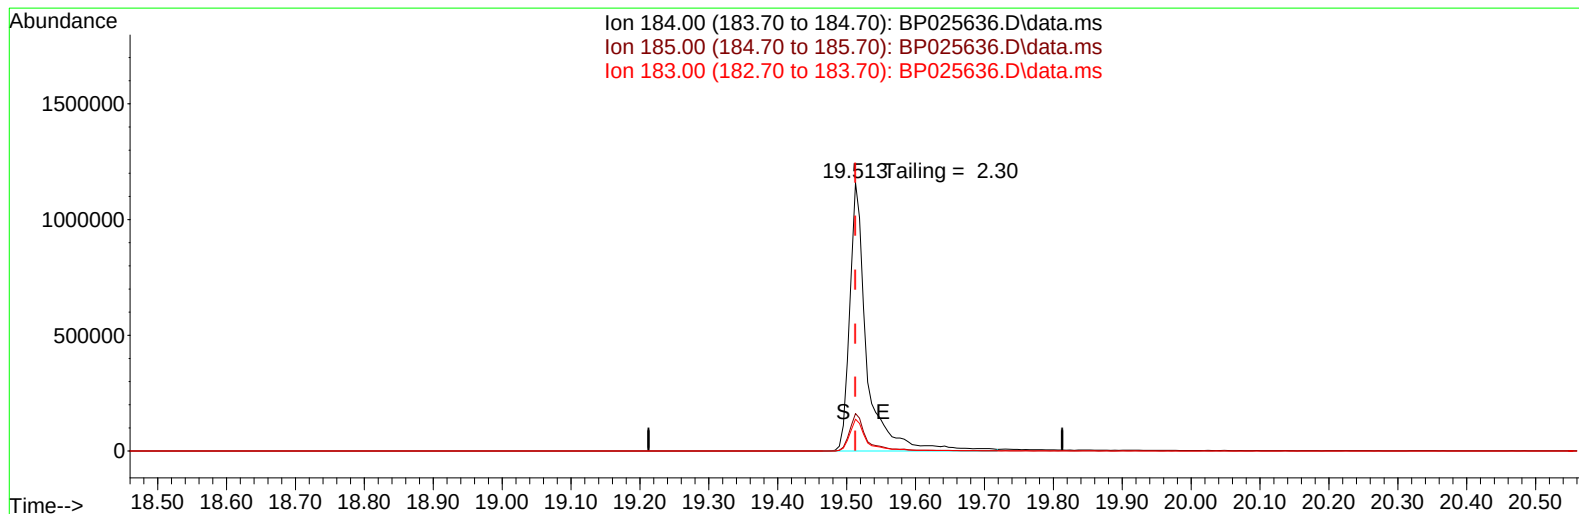

TIC: BP025636.D\data.ms

(77) Benzidine**19.513min (+ 0.000) 750466.85 ng****response 1229369**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.96
183.00	11.80	11.89
0.00	0.00	0.00