
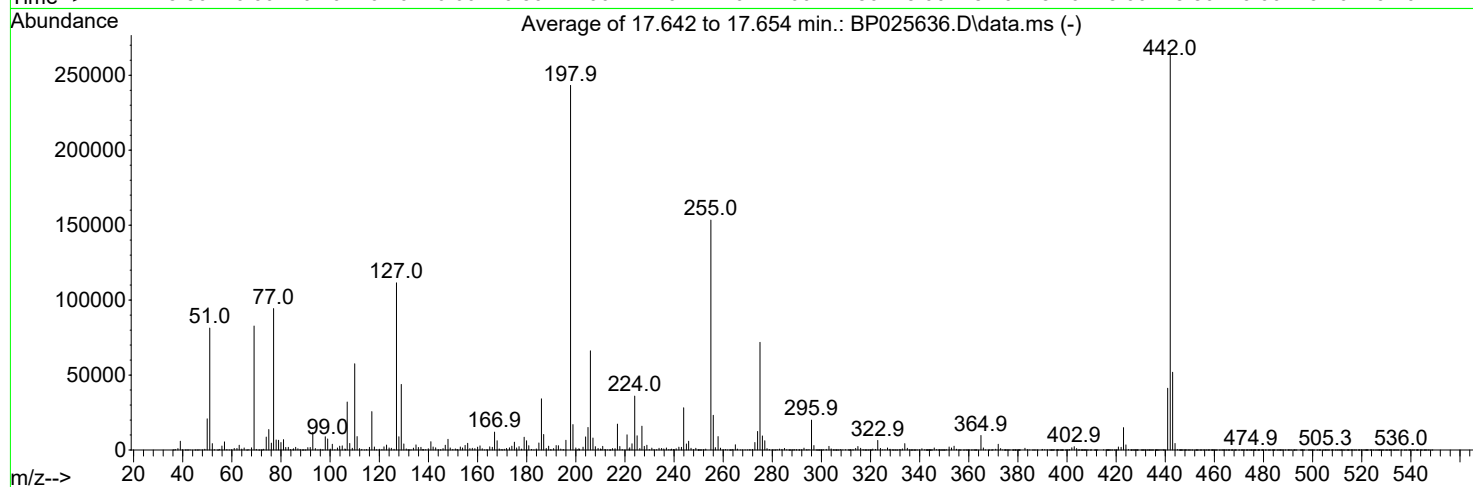


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090225\
Data File : BP025636.D
Acq On : 02 Sep 2025 13:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 14 18:14:31 2025

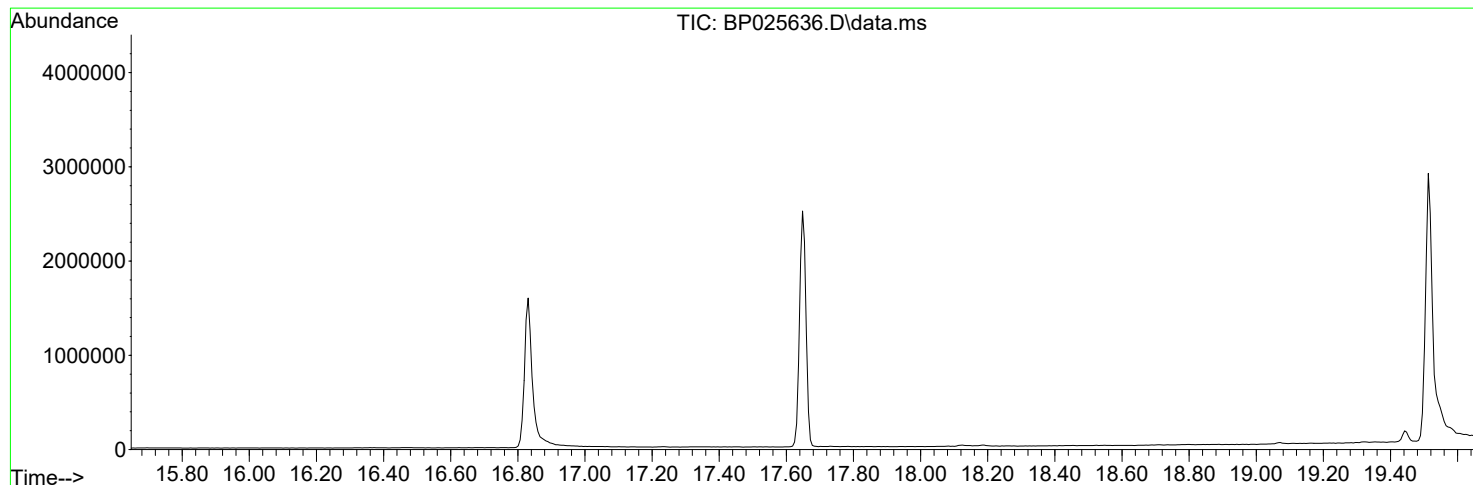

AutoFind: Scans 2500, 2501, 2502; Background Corrected with Scan 2492

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.9	1538	PASS
69	69	100	100	100.0	82745	PASS
70	69	0.00	2	0.5	454	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	243250	PASS
199	198	5	9	7.0	17026	PASS
365	198	1	100	4.0	9686	PASS
441	443	0.01	150	79.3	41172	PASS
442	442	100	100	100.0	263403	PASS
443	442	15	24	19.7	51916	PASS

DDT Breakdown


Date	Instrument Name	DFTPP Data File
9/2/2025	BNA_P	<u>BP025636.D</u>
Compound Name	Response	Retention Time
DDT	1017018	20.807
DDD	29323	20.348
DDE	4771	19.819
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
34094	1051112	3.24

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090225\
Data File : BP025636.D
Acq On : 02 Sep 2025 13:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 02 14:38:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

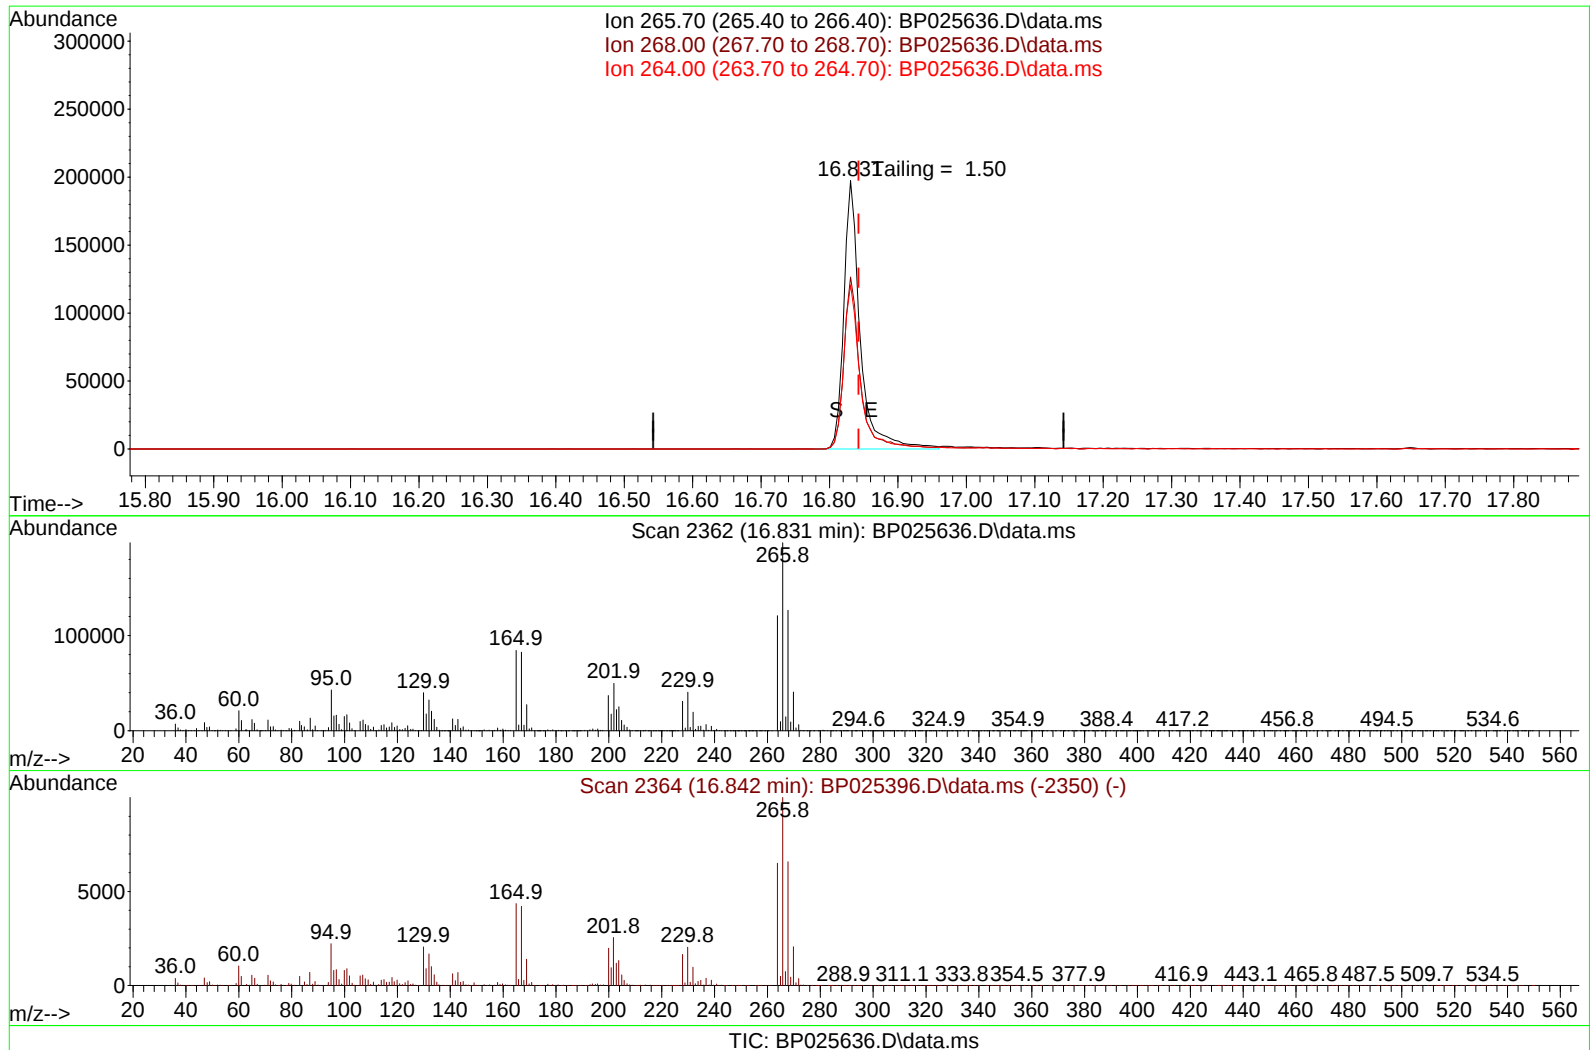

TIC: BP025636.D\data.ms

(70) Pentachlorophenol (C)

16.831min (-0.012) 2157219.78 ng




response 312500

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	64.08
264.00	65.00	61.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090225\
Data File : BP025636.D
Acq On : 02 Sep 2025 13:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 02 14:38:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

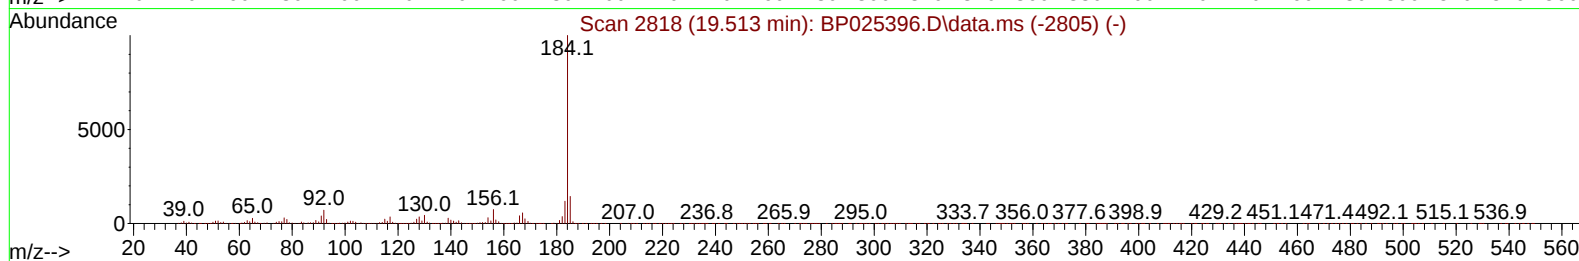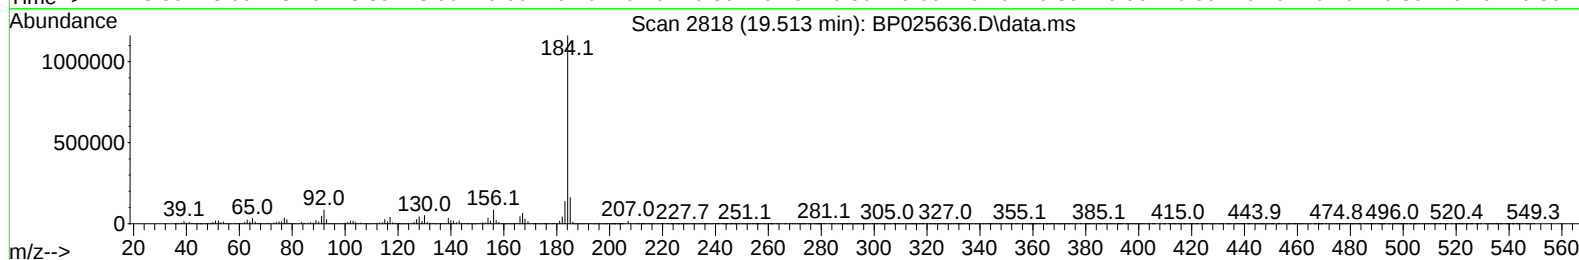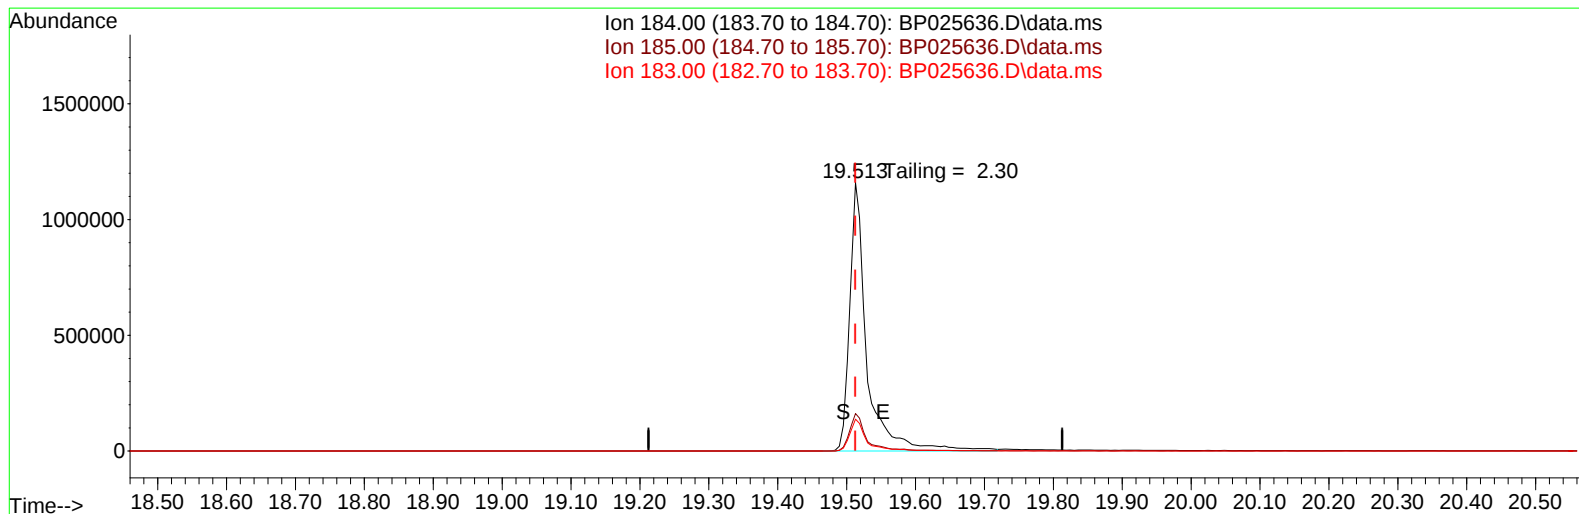

TIC: BP025636.D\data.ms

(77) Benzidine

19.513min (+ 0.000) 750466.85 ng

response 1229369

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.96
183.00	11.80	11.89
0.00	0.00	0.00