


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP090419\
 Data File : BP000051.D
 Acq On : 04 Sep 2019 08:55
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP083019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 30 17:47:17 2019

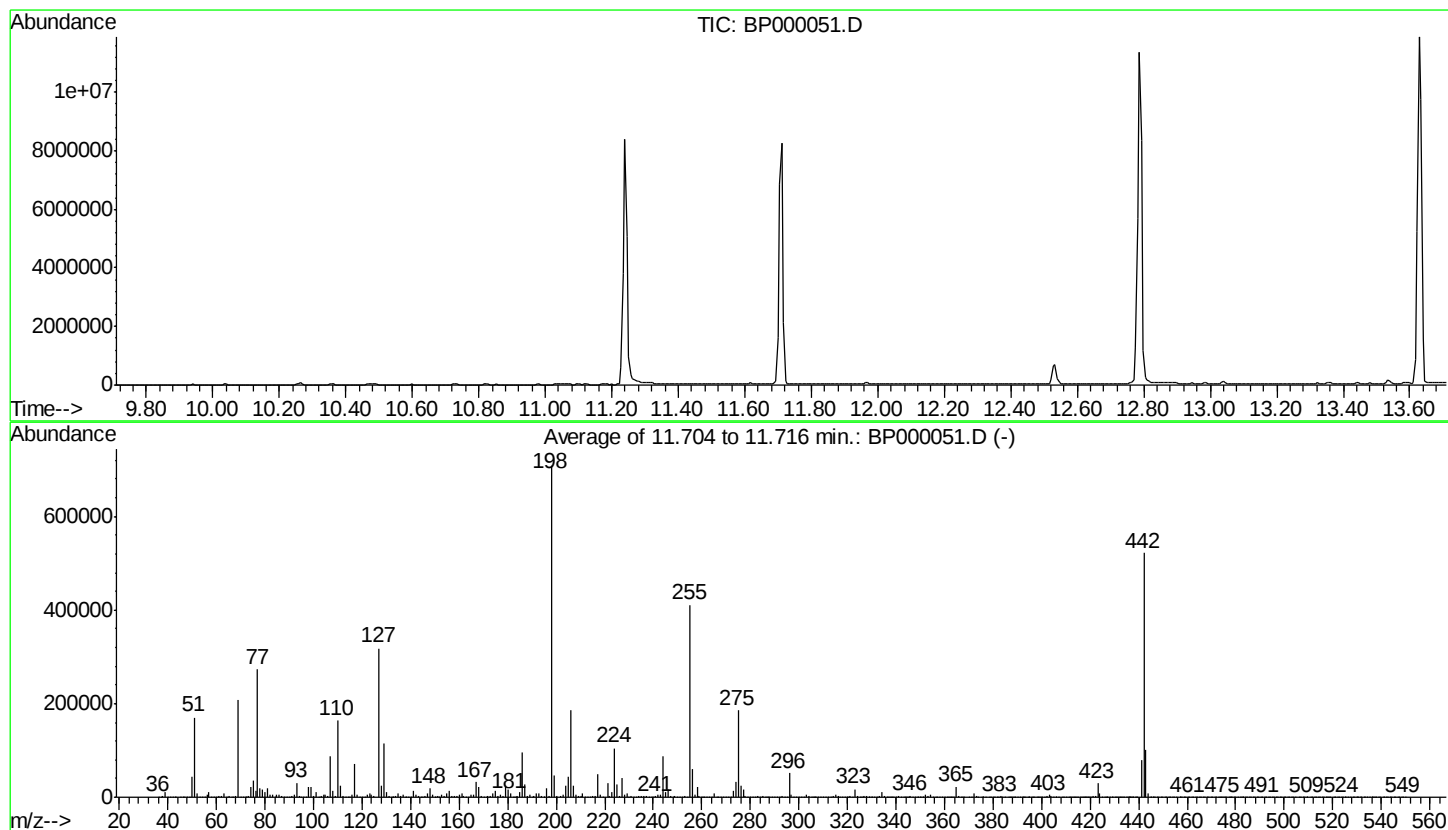

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1627

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.0	170246	PASS
68	69	0.00	2	1.8	3682	PASS
69	198	0.00	100	29.4	208204	PASS
70	69	0.00	2	0.5	1127	PASS
127	198	10	80	44.9	317885	PASS
197	198	0.00	2	0.2	1655	PASS
198	198	100	100	100.0	708565	PASS
199	198	5	9	6.7	47540	PASS
275	198	10	60	26.2	185392	PASS
365	198	1	100	3.2	22589	PASS
441	198	0.01	100	11.3	80138	PASS
442	198	50	100	73.7	522197	PASS
443	442	15	24	19.2	100469	PASS